



Noradrenaline ELISA Kit

(For Human)

Enzyme Immunoassay for the quantification of Noradrenaline in plasma samples.

Catalog number: ARG80474

For research use only. Not for use in diagnostic procedures.

TABLE OF CONTENTS

SECTION	Page
PRINCIPLE OF THE ASSAY	3
MATERIALS PROVIDED & STORAGE INFORMATION.....	3
MATERIALS REQUIRED BUT NOT PROVIDED.....	5
TECHNICAL HINTS AND PRECAUTIONS	5
SAMPLE COLLECTION & STORAGE INFORMATION	5
REAGENT PREPARATION	6
ASSAY PROCEDURE	6
CALCULATION OF RESULTS.....	9
EXAMPLE OF TYPICAL STANDARD CURVE.....	10
QUALITY ASSURANCE	10

MANUFACTURED BY:

Arigo Biolaboratories Corporation

Address: No. 22, Ln. 227, Gongyuan Rd., Hsinchu City 300, Taiwan

Phone: +886 (3) 562 1738

Fax: +886 (3) 561 3008

Email: info@arigobio.com

Noradrenaline ELISA Kit ARG80474

PRINCIPLE OF THE ASSAY

This is an Enzyme Immunoassay for the quantification of Noradrenaline in plasma samples.

This assay employs the competitive quantitative enzyme immunoassay technique. Noradrenaline are first extracted by using a cis-diol-specific affinity gel, acylated and derivatized enzymatically.

The antigen has been pre-coated onto a microtiter plate. Extracted and derivatized controls, standards or samples and the solid phase bound analytes compete for a fixed number of antiserum binding sites. When the system is in equilibrium, free antigen and free antigen-antiserum complexes are removed by washing. Anti-rabbit IgG conjugated to Peroxidase is added to each well and incubated. After washing away any unbound antibody conjugate, a substrate solution (TMB) is added to the wells and color develops in inverse-proportion to the amount of Noradrenaline present in the samples. The color development is stopped by the addition of STOP solution and the intensity of the color is measured at a wavelength of 450nm \pm 2nm. The concentration of Noradrenaline in the sample is then determined by comparing the O.D of samples to the standard curve.

MATERIALS PROVIDED & STORAGE INFORMATION

Store the unopened kit at 2-8 °C. Use the kit before expiration date.

Component	Quantity	Storage information
Noradrenaline- Normetanephrine	12 strips X 8 wells	4°C

Noradrenaline ELISA Kit ARG80474

coated microplate		
Adhesive foil	4 pieces	RT
50X Wash Buffer	20ml	4°C
Anti-rabbit IgG- peroxidase conjugate	12ml (Ready-to-use)	4°C
TMB substrate	12ml (Ready-to-use)	4°C (Protect from light)
STOP solution	12ml (Ready-to-use)	4°C
Standard A-F	4ml each (Ready-to-use)	4°C
Noradrenaline Antiserum	6ml (Ready-to-use)	4°C
Adjustment Buffer	1 X 4ml (Ready-to-use)	4°C
Acylation Buffer	20ml (Ready-to-use)	4°C
Acylation Reagent	3ml (Ready-to-use)	4°C
TE Buffer	4ml (Ready-to-use)	4°C
Coenzyme (S-adenosyl- L-methionine)	2ml (Ready to use)	4°C
Enzyme (COMT)	4 X 1ml (Lyophilized)	4°C
Extraction Plate (coated with boronate affinity gel)	2 X 48 wells (Ready-to-use)	4°C
Control 1	4ml (Ready-to-use)	4°C
Control 2	4ml (Ready-to-use)	4°C
Microtiter Plate for Enzyme Conversion	12 strips X 8 wells	4°C
Hydrochloric Acid	20ml (Ready-to-use)	4°C

MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of measuring absorbance at 450nm
- Pipettes and pipette tips
- Deionized or distilled water
- Automated microplate washer (optional)

TECHNICAL HINTS AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Store the kit at 4°C at all times.
- Briefly spin down the antibody conjugate concentrate and HRP-Streptavidin concentrate before use.
- If crystals are observed in the 50X Wash buffer, warm to RT (not more than 50°C) until the crystals are completely dissolved.
- Ensure complete reconstitution and dilution of reagents prior to use.
- It is highly recommended that the standards, samples and controls be assayed in duplicates.
- Change pipette tips between the addition of different reagent or samples.

SAMPLE COLLECTION & STORAGE INFORMATION

Plasma - Collect plasma using EDTA as an anticoagulant. Do not use haemolytic or lipemic samples. Assay immediately (up to 6 hours at 2-8 °C), or aliquot and store samples at ≤ -20 °C (up to 6 months). Avoid repeated

Noradrenaline ELISA Kit ARG80474

freeze-thaw cycles. Avoid exposure to direct sunlight.

A plasma volume between 100 μ l - 600 μ l is needed per single determination. If a plasma volume < 600 μ l is used, distilled water has to be added to a final volume of 600 μ l and this prediluted sample has to be used for the extraction procedure. The sample predilution has to be considered in the calculation of results.

REAGENT PREPARATION

- **1X Wash buffer:** Dilute 50X Wash buffer into distilled water to yield 1X Wash buffer. Storage: up to 6 months at 4-8°C.
- **Enzyme solution:** Reconstitute the lyophilized “Enzyme” with 1ml of distilled water and mix well. Add 0.3ml coenzyme followed by 0.7ml Adjustment buffer. The total volume of Enzyme solution is 2ml. Prepare fresh prior to assay (not more than 10-15 minutes in advance). Discard unused Enzyme solution.

ASSAY PROCEDURE

Sample Preparation, Extraction and Acylation, Enzymatic Conversion

1. Pipette 30 μ l of standards, controls, urine samples and 600 μ l of plasma samples into the appropriate wells of the Extraction Plate.
2. Add 500 μ l of distilled water to wells with standards, controls and urine samples.
3. Add 25 μ l TE Buffer to all wells.
4. Cover plate and incubate for 60 mins at RT on shaker (~600rpm)

Noradrenaline ELISA Kit ARG80474

5. Remove foil, discard and blot dry by tapping the inverted plate on absorbent material. Wash each well with 1ml wash buffer and shake for 5 mins at RT on a shaker (600rpm). Blot dry by tapping the inverted plate on absorbent material.
6. Repeat wash as step 5. Discard and blot dry by tapping the inverted plate on absorbent material.
7. Add 150µl Acylation Buffer into all wells.
8. Add 25µl Acylation Reagent into all wells.
9. Incubate for 20 mins at RT on shaker (~600rpm)
10. Remove foil, discard and blot dry by tapping the inverted plate on absorbent material. Wash each well with 1ml wash buffer and shake for 5 mins at RT on a shaker (600rpm). Blot dry by tapping the inverted plate on absorbent material.
11. Repeat wash as step 10.
12. Add 200µl Hydrochloric Acid into all wells.
13. Cover plate and incubate for 10 mins at RT on shaker (~600rpm)
- 14. Remove foil, do not decant the supernatant!**
15. 190µl of supernatant is needed for the subsequent enzymatic conversion.
16. For enzymatic conversion, pipette 190µl of the extracted standards, controls and samples into the respective wells of the microtiter plate.
17. Add 50µl of Enzyme Solution to all wells.
18. Cover plate with adhesive foil. Shake 1 min at RT on a shaker.
19. Incubate for 2 hours at 37°C. Use 10µl for subsequent Dopamine ELISA assay.

Noradrenaline ELISA procedure

1. Remove excess microtiter strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal it.
2. Add 10 μ l of the extracted standards, controls and samples into the appropriate wells of Noradrenaline Microtiter Strips.
3. Add 50 μ l of Noradrenaline Antiserum into wells.
4. Cover plate with Adhesive foil and incubate for 1 min at RT on a shaker (600rpm).
5. Incubate for 15-20 hours (overnight) at 2-8°C.
6. Remove the foil and discard. Aspirate each well and wash, repeating the process 4 times for a total 5 washes. Wash by filling each well with 1 \times Wash Buffer (350 μ l) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
7. Add 100 μ l of Anti-rabbit IgG-peroxidase conjugate into wells.
8. Incubate for 30 mins at RT on a shaker (600rpm).
9. Aspirate each well and wash as step 6.
10. Add 100 μ l of TMB substrate solution into each well. Incubate for 20-30 mins at RT with shaking (600rpm). Avoid exposure to light.
11. Add 100 μ l of Stop Solution to each well and shake lightly to ensure homogeneous mixing.

CALCULATION OF RESULTS

1. Calculate the average absorbance values for each set of standards, controls and samples.
2. Using linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
3. Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
4. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
5. The concentrations of undiluted samples and controls can be read directly from the standard curve.
6. Concentration of diluted samples: If plasma volume of <600µl is used, the concentration read from the standard curve has to be multiplied by a volume factor:

$$\text{Volume factor} = 600\mu\text{l} / \text{used plasma volume } (\mu\text{l})$$


Noradrenaline ELISA Kit ARG80474

7. Refer to the table below for molar conversion:

	Concentration of standards					
Standard	A	B	C	D	E	F
Noradrenaline (pg/ml)	0	80	240	800	3200	12800
Noradrenaline (pmol/L)	0	473	1418	4728	18912	75648
Conversion	Noradrenaline (ng/ml) x 5.91 = Noradrenaline (nmol/L)					

EXAMPLE OF TYPICAL STANDARD CURVE

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

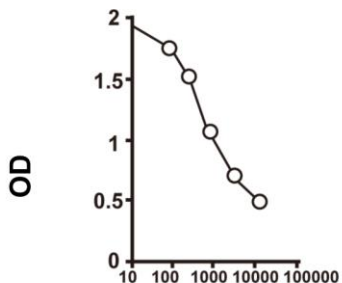

Competitive ELISA:
Noradrenaline Concentration (pg/ml)

QUALITY ASSURANCE

Sensitivity

NAD: 35 pg/ml

Noradrenaline ELISA Kit ARG80474

Assay Range

NAD: 80-12800 pg/ml

Specificity

No significant cross-reactivity was found for the following factors:

Adrenaline, Dopamine, Metanephrine, Normetanephrine, 3-Methoxytyramine, 3-Methoxy-4-hydroxyphenylglycol, Tyramine, Phenylalanine, Caffeinic acid, L-DPOA, Homovanillic acid, 3-Methoxy-4-Hydroxymandelic acid.

Intra-assay and Inter-assay precision

The CV value of intra-assay precision was 8.4-15.6%.

Recovery

104.8-125.6%

Linearity

84-123%