

# Exendin-4 (Heloderma Suspectum) - Fluorescent EIA Kit

Catalog#	Standard size	Price	Order
FEK-070-94	1 kit	\$460.00	<input type="button" value="ORDER"/>

## Product description

## More information

[Exendin-4, Research Abstracts, Kits Standard Curves, Sequences, etc.](#)

[Neuron Function Modulation](#)

**Protocol** [Fluorescent EIA Kit \(PDF\)](#)

\*Please Note: To reduce the background level for FEK-070-94, refrain from adding EDTA to samples.

**Sample Preparation** [Blood collection](#)  
[Plasma extraction](#)  
[Tissue extraction](#)  
[CSF extraction](#)

**Catalog #** FEK-070-94

**Standard Size** 96 well


**Sensitivity** Minimum Detectable Concentration = 11.2 pg/ml

**Range** 0-10000 pg/ml

**Linear Range** 11.2-273 pg/ml

<b>Cross Reactivity</b>	<b>Peptide</b>	<b>%Cross-reactivity</b>
	Exendin-4	100
	Exendin-3 (9-39)-NH <sub>2</sub>	100
	Exendin-4 (3-39)	100
	Lixisenatide	80
	Glucagon (Human, Rat, Mouse, Porcine, Bovine)	0
	GLP-1(7-36)-NH <sub>2</sub> (Human, Rat, Mouse)	0
	Oxyntomodulin (Human, Rat, Mouse)	0
	GLP-2 (Human)	0
	GLP-1(7-37) (Human, Rat, Mouse)	0

Standard  
Curve Image

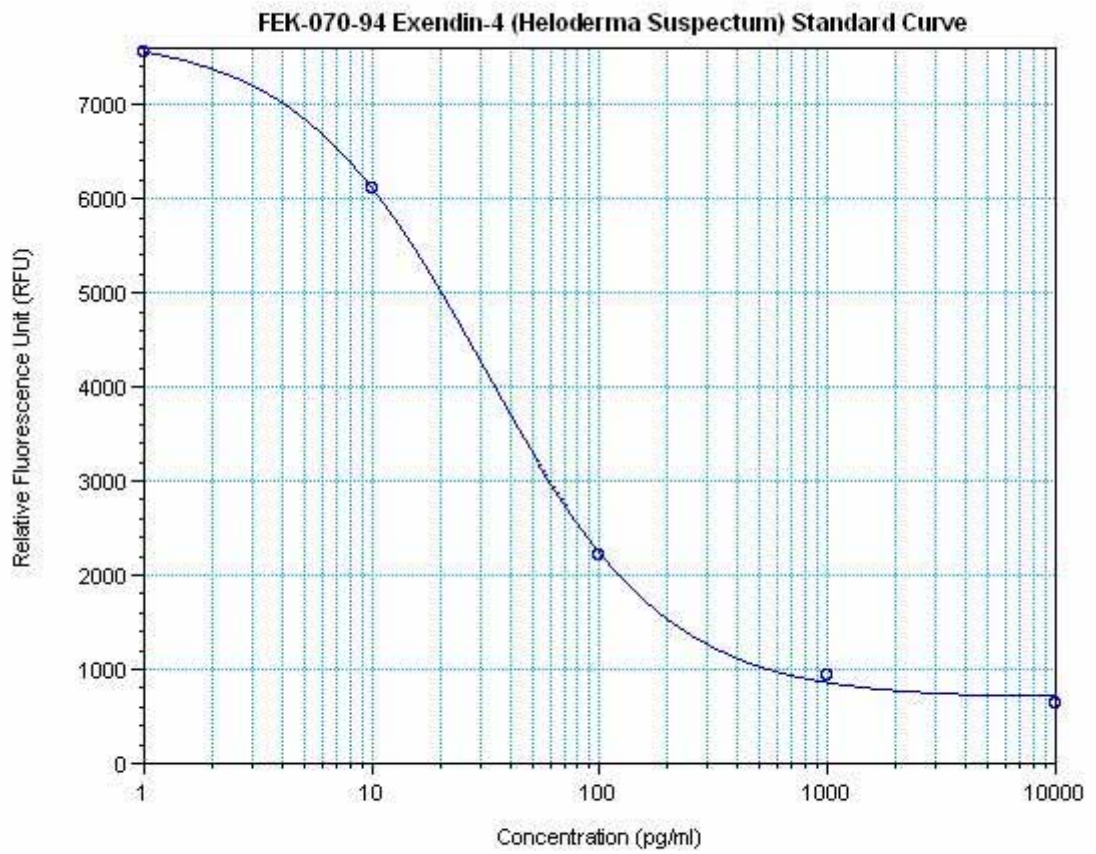

4-P Fit:  $y = (A - D) / (1 + (x/C)^B) + D$