



SensoLyte[®] Anti-Mouse/Rat β -Amyloid (1-40) Quantitative ELISA *Colorimetric*

Revision : 1.2

Last updated : 02/05/2020

Catalog #	AS-55553
Kit Size	One 96-well strip plate

This kit is optimized to detect mouse/rat beta-Amyloid (1-40) peptide in mouse/rat brain lysate, cerebrospinal fluid, or plasma. Wells are pre-coated with monoclonal anti-beta-Amyloid (1-40) specific capture antibodies and blocked with a proprietary blocking solution. The amount of mouse/rat beta-Amyloid (1-40) is quantified using ELISA. Ample materials and reagents are provided to perform 96 assays.

- **Convenient Format**
 - Pre-coated and pre-blocked 96-well strip plate
 - Ready-to-use substrate solution and other assay components
 - One step assay (samples and detection antibodies are added simultaneously)
 - 1 hour assay time at room temperature (excluding incubation)
- **High Sensitivity**
 - Detects as low as 2 pg/ml (13 fmoles/ml) of mouse/rat beta-Amyloid (1-40) in brain lysate
- **Broad Dynamic Range**
 - 3.9-250 pg/ml of mouse/rat beta-Amyloid (1-40) peptide

Kit Components and Handling

Component	Description	Quantity
Component A	Mouse monoclonal anti-beta-Amyloid (1-40) coated plate	12 x 8-well strips
Component B	Mouse/rat beta-Amyloid (1-40) Peptide Standard (lyophilized)	1 μ g
Component C	1 X Sample Dilution Buffer	60 ml
Component D	10 X Wash Buffer	30 ml
Component E	TMB Color Substrate Solution	10 ml
Component F	Stop Solution	10 ml
Component G	Peptide Standard Reconstitution Buffer	1 ml
Component H	Detection Antibody (Rabbit anti-Mouse/Rat beta-Amyloid-HRP)	50 μ l
Component I	1 X Detection Antibody Dilution Buffer	10 ml
Component J	Adhesive Plate Covers	2 pieces

Other Materials Required (but not provided)

- Microplate reader: Capable of reading absorbance at 450 nm
- Rocking platform or shaker
- Strip ejector (to eject strips for future assay if not all strips are used in one experiment)
- Plate washer (optional)

Shipment and Storage

- Kit is shipped on blue ice. Upon receipt, store all kit components at 2-8 °C for up to 6 months
- Reconstituted Peptide Standard (Component B) must be stored at -80 °C in small aliquots

For research use only! Not for diagnostic use!

Introduction

Alzheimer's Disease (AD) is the most common neurodegenerative disorder in elderly people. It has been demonstrated that AD has biological causes and is characterized by the presence of senile plaques and neurofibrillary tangles mainly in cerebral cortex and hippocampus brain regions.¹⁻⁵ Beta-Amyloid (1-40) (A β 40) and beta-Amyloid (1-42) (A β 42) are the main components of the above plaques; however, other forms of beta-Amyloid peptides are also present. Both peptides are cleaved from the Amyloid Precursor Protein (APP) by β -secretase and γ -secretase enzymes.^{2,3,5} Many studies suggest that A β 42 or/and A β 43 are required to initiate formation of amyloid plaques and neurofibrils that leads to the neurodegeneration,¹⁻⁵ while A β 40 is less neurotoxic.

The SensoLyte[®] beta-Amyloid (1-40) Quantitative ELISA Kit (Mouse/Rat) provides a convenient and quantitative assay for determining mouse/rat A β 40 amount in cell and tissue lysate as well as in body fluids. Compared to other anti-A β 40 ELISA kits on the market, it takes less time to run this assay. HRP conjugated detection antibody in this kit is added simultaneously with the samples and standards during the assay. This eliminates extra incubation and washing steps and makes this kit a one-step procedure for A β 40 quantification.

Experimental Protocol

Please Note:

- a) Bring kit components to room temperature before starting the assay
- b) Spin down all components with volume less than 100 μ l before use
- c) Mix the Washing Buffer (Component D) to dissolve any precipitated salt

1 ELISA Protocol:

- 1.1 Reconstitute mouse/rat beta-Amyloid (1-40) Standard (Component B) with 1 ml of Peptide Standard Reconstitution Buffer (Component G). Allow peptide to hydrate for ten minutes. Mix gently by inverting. Aliquot the reconstituted standard in 100 μ l per vial (vials are not provided with the kit), label, and save unused A β 40 standard at -80°C . We recommend using glass vials such as borosilicate for storage of the reconstituted standard to avoid absorption of A β 40 to plastic surfaces. **Do not reuse reconstituted standard once it is thawed.**
- 1.2 Arrange and label strips (Component A) based on the number of wells for standards and samples. Although diluted standards and samples can be run as single points, duplicates are recommended. Instructions for preparing brain lysate are provided in the **Appendix** section. Place unused strips into the supplied bag, seal completely, and store at 4°C .
- 1.3 Prepare serial dilution of the A β 40 standard immediately before use. Refer to the table below.

Step	Concentration, pg/ml	A β 40 Standard (Component B)	Sample Dilution Buffer (Component C)
1	1,000,000	<i>Prepare as described in 1.1</i>	
2	10,000	10 μ l from step 1	990 μ l
3	250	25 μ l from step 2	975 μ l
4	125	500 μ l from step 3	500 μ l
5	62.5	500 μ l from step 4	500 μ l
6	31.25	500 μ l from step 5	500 μ l
7	15.625	500 μ l from step 6	500 μ l
8	7.8125	500 μ l from step 7	500 μ l
9	3.91	500 μ l from step 8	500 μ l

- 1.4 Dilute Detection Antibody(Component H)200 fold in Detection Antibody Dilution Buffer (Component I).Prepare 50 μ l of the above antibody solution for each well to be run in the assay. One strip requires 0.5 ml of the diluted detection antibody solution.

- 1.5 Add 100 µl per well of the diluted Aβ40 standards (Starting with Step 3 from 1.3) in duplicates including blank. We recommend diluting plasma at 1:20 dilution ratio and CSF at 1:4 dilution ratio with 1 X Sample Dilution Buffer to avoid sample matrix effects. For brain lysate, it is recommended to use 1:40 dilution ratio. In addition, protease inhibitor cocktail with PMSF must be added to all samples to avoid protein degradation (A recipe example is provided in the **Appendix** section).
- 1.6 Add 100 µl of the diluted samples into the appropriate wells.
- 1.7 Add 50 µl of the diluted detection antibody solution (from Step 1.4) into each well to be assayed, apply Adhesive Plate Cover (Component J), and incubate plate overnight at 4 °C. **Protect wells from the light.**
- 1.8 Prepare 1X working wash buffer by diluting the 10 X Wash Buffer (Component D) with deionized H₂O.
- 1.9 After plate incubation, aspirate the wells and wash them with 350 µl/well of 1x wash buffer 6-7 times. Allow 20 seconds soaking time before emptying the wells between washes. Pat dry the plate using a paper towel and clean outside of wells with non-abrasive paper to ensure accurate optical reading.
- Insufficient washing will increase background reading.**
- 1.10 Add 100 µl of the TMB Color Substrate Solution (Component E) into each well. Tap plate gently and incubate at room temperature until blue gradient is clearly observed across the wells (5- 15 min). It may be necessary to adjust color development time so that absorbance values will fall within the detection range. Samples may require further dilution if Aβ40 concentration is too high.
- 1.11 Add 50 µl of the Stop Solution (Component F) into each well and tap plate gently (blue color will turn to yellow). Measure absorbance (OD) at 450 nm using a microplate absorbance reader within 20 minutes after adding the Stop Solution.

2. Calculate the concentration of mouse/rat Aβ40 in samples.

- 2.1 Determine the average values (if replicates are used) for the Aβ40 standard and sample absorbance readings. Plot calibration curve using Linear Regression curve-fit. R² should be higher than 0.98. There should be at least 5 standard concentrations in the calculation to ensure statistical significance. The reading for the highest standard concentration (250 pg/ml) can be excluded from the curve if the signal is too strong.
- 2.2 Choose absorbance values for the diluted samples that are within the range used in the Aβ40 standard curve, and calculate the concentration of mouse or rat Aβ40 in the tested sample(s). Calculated concentrations must be multiplied by the sample dilution factor.
- 2.3 Typical Aβ40 Standard Curve:

Please note, standard curve data results are influenced by operator variability, temperature, pipetting techniques, etc. Therefore, it is important to generate a new standard curve for each assay that is performed.

Note: 1) Standards were run in duplicates, blank value was subtracted, and the 250 pg/ml point was excluded from the standard curve graph.

2) Aβ42 data is shown for cross-reactivity purpose.

Aβ40, pg/ml	OD @ 450 nm, Aβ40	OD @ 450 nm, Aβ42
250	2.769	0.043
125	1.964	0.023
62.5	1.124	0.011
31.25	0.587	0.008
15.6	0.282	0.011
7.8	0.14	0.003
3.9	0.065	0.015
0	0	0

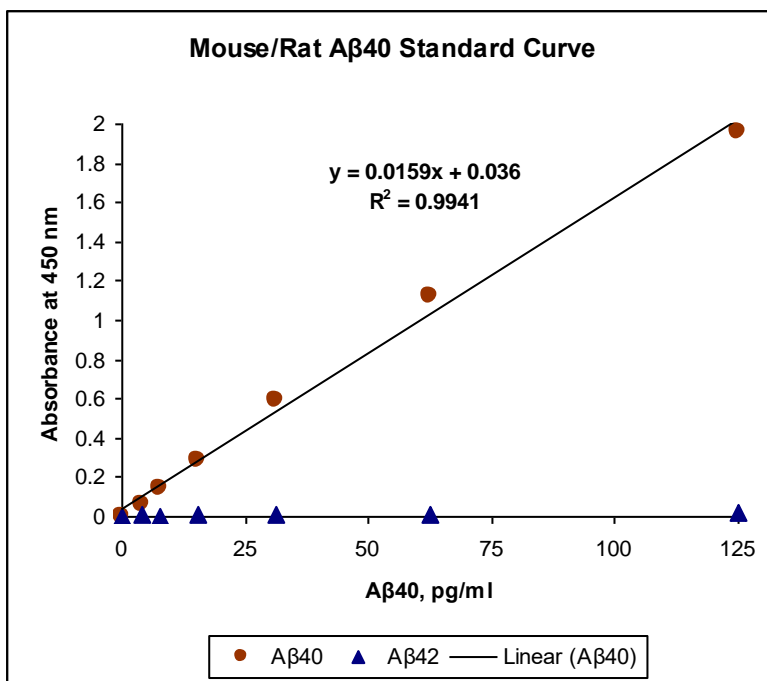


Figure 1. An example of the mouse/rat Aβ40 ELISA standard curve.

3. Kit Performance.

3.1 Aβ40 Recovery Test:

Mouse/rat Aβ40 was added to the diluted mouse brain lysate (1:40 dilution ratio) and assayed using the kit

Specimen	Theoretical Value, (pg/ml)	Measured Value, (pg/ml)	% Recovery
Brain Lysate	40	41	102
Brain Lysate	5	5.05	101

Note: 1. Mouse brain lysate was diluted 40 times with Sample Dilution Buffer
2. Each spiked value was assayed 10 times

3.2 Intra-Assay Variation Test:

Measurement Value, (pg/ml)	Standard Deviation	Coefficient of Variation	n
5	0.39	7.7	10

3.3 Cross Reactivity Test:

Peptide	Cross Reactivity, %
Mouse/Rat Aβ40	100
Mouse/Rat Aβ42	<1.2
Mouse/Rat Aβ37	<0.1
Mouse/Rat Aβ28	<0.1

Note: All tested peptides were added at 125 pg/ml concentration.

Appendix

1. Buffer composition for brain homogenate:

5M Guanidine HCl
50 mM Tris HCl, pH=8.0

Mix 800 µl of the above solution with 100 mg of brain sample in a Dounce homogenizer placed on ice. Homogenize the tissue thoroughly and incubate at room temperature for 3-4 hours with mixing. Guanidine-HCl brain homogenates are stable at 4°C for several weeks and can be freeze-thawed many times without degradation of beta-Amyloid peptides.

Dilute brain homogenate with "Sample Dilution Buffer" (Component C) for the assay. We recommend 1:40 dilution to start with for mouse brain homogenate. User should determine the optimal dilution factor. Transgenic mouse brain lysates require higher dilution factor due to the high concentration of Aβ40 peptide present in the brain. **Guanidine-HCl concentration higher than 0.125M will result in a significant loss of signal in the assay.**

2. Protease Inhibitor Cocktail Recipe (100 X concentrate)

Aprotinin 0.4 mg
Leupeptin 2 mg
Deionized H₂O 900 µl

Dissolve 0.1 mg of Pepstatin A in 100 µl of methanol and mix with the above solution.
Aliquot and store cocktail at -80 °C.

3. 100 mM PMSF Solution (100 X concentrate):

Dissolve 174 mg of PMSF in 10 ml of pure isopropanol, aliquot, and store at -80°C.
Add to the protease inhibitor cocktail (1mM final concentration) immediately before use.

References:

1. Levites Y. et al., J. Clinical Investigations 116(1): 193-201: 2006
2. Broersen K. et al., Alzheimer's Research and Therapy 2: 1-14, 2010
3. Zhang Yun-Wu, et al., Molecular Brain 4: 1-13: 2011
4. Koehling T., et al., Int. J. Alzheimer's Disease, 2010
5. Bobba A., et al., Int. J. Alzheimer's Disease, 2010