

Anti-Ovalbumin IgG₁ (mouse) EIA Kit

Item No. 500830



Customer Service 800.364.9897 * Technical Support 888.526.5351

www.caymanchem.com

TABLE OF CONTENTS

GENERAL INFORMATION	3	Materials Supplied
	4	Precautions
	4	If You Have Problems
	4	Storage and Stability
	4	Materials Needed but Not Supplied
INTRODUCTION	5	Background
	5	About This Assay
	6	Description of Immunometric EIAs
PRE-ASSAY PREPARATION	7	Buffer Preparation
	7	Sample Preparation
ASSAY PROTOCOL	8	Preparation of Assay-Specific Reagents
	9	Plate Set Up
	10	Performing the Assay
ANALYSIS	12	Calculations
	12	Performance Characteristics
RESOURCES	17	Troubleshooting
	17	References
	18	Related Products
	18	Warranty and Limitation of Remedy
	19	Plate Template
	20	Notes

GENERAL INFORMATION

Materials Supplied

Item Number	Item	96 wells Quantity/Size
400830	Goat Anti-Mouse IgG ₁ HRP Detection Antibody	1 vial/1.5 ml
400832	Ovalbumin Precoated 96-Well Strip Plate	1 plate
400834	Anti-Ovalbumin IgG ₁ (mouse) EIA Standard	1 vial/200 ng
400054	Immunoassay Buffer B Concentrate (10X)	2 vials/10 ml
400062	Wash Buffer Concentrate (400X)	1 vial/5 ml
400035	Polysorbate 20	1 vial/3 ml
400074	TMB Substrate Solution	1 vial/12 ml
10011355	HRP Stop Solution	1 vial/12 ml
400012	96-Well Cover Sheet	3 covers

If any of the items listed above are damaged or missing, please contact our Customer Service department at (800) 364-9897 or (734) 971-3335. We cannot accept any returns without prior authorization.



WARNING: This product is for laboratory research use only: not for administration to humans. Not for human or veterinary diagnostic or therapeutic use.

Precautions

Please read these instructions carefully before beginning this assay.

The reagents in this kit have been tested and formulated to work exclusively with Cayman's Anti-Ovalbumin IgG₁ (mouse) EIA Kit. This kit may not perform as described if any reagent or procedure is replaced or modified. The Stop Solution provided with this kit is an acid solution. Please wear appropriate personal protection equipment (*e.g.*, safety glasses, gloves, and lab-coat) when using this material.

For research use only. Not for human or diagnostic use.

If You Have Problems

Technical Service Contact Information

Phone:	888-526-5351 (USA and Canada only) or 734-975-3888
Fax:	734-971-3641
Email:	techserv@caymanchem.com
Hours:	M-F 8:00 AM to 5:30 PM EST

In order for our staff to assist you quickly and efficiently, please be ready to supply the lot number of the kit (found on the outside of the box).

Storage and Stability

This kit will perform as specified if stored as directed at 4°C and used before the expiration date indicated on the outside of the box.

Materials Needed But Not Supplied

1. A plate reader capable of measuring absorbance at 450 nm.
2. Adjustable pipettes and a repeating pipettor.
3. A source of pure water; glass distilled or deionized water is acceptable
4. Materials used for **Sample Preparation** (see page 7).

INTRODUCTION

Background

Immunization of mice with chicken egg albumin (ovalbumin/OVA) in a precipitate complex with aluminum hydroxide (alum) is a highly effective means of inducing a potent TH2-mediated immune response.¹⁻⁶ OVA/alum immunized mice produce anti-OVA antibodies predominantly of the IgG₁ and IgE isotypes that mediate tissue-specific effector functions in multiple mouse models of chronic inflammation, including allergic asthma, allergic rhinitis, and cutaneous hypersensitivity.¹⁻⁴

When using one of these models, it is often desirable to measure anti-OVA antibody levels in the plasma or serum to determine the effectiveness of the immunization, the activity of a drug, or the effect of a specific gene deletion. IgG₁ is the predominant anti-OVA immunoglobulin isotype found in the serum or plasma of mice immunized with OVA/alum; the plasma concentration of OVA-specific IgG₁ is typically 1,000-fold greater than that of OVA-specific IgE.¹ Therefore, the measurement of anti-OVA IgG₁ is a commonly used method of assessing the magnitude of this TH2 immune response.

About This Assay

Cayman's Anti-Ovalbumin IgG₁ (mouse) EIA Kit is an immunometric (*i.e.*, 'sandwich') assay which can be used to measure anti-ovalbumin of the IgG₁ isotype in mouse plasma and serum without prior sample purification. Affinity-purified anti-ovalbumin IgG₁ isolated from the plasma of mice immunized with OVA/alum is used as the standard. The standard curve spans the range of 1.56-200 ng/ml, with an LLOQ of 1.56 ng/ml.

Description of Immunometric EIAs

Each well of the microwell plate supplied in the kit has been coated with ovalbumin. Antibodies specific for ovalbumin, if present in the biological fluid sample, will bind to the immobilized ovalbumin. A detection antibody recognizing mouse IgG₁ is added to the well. This Goat Anti-mouse IgG₁ is labeled with HRP, allowing quantitation of the autoantibody. Addition of the HRP Substrate 3,3',5,5'-tetramethylbenzidine (TMB), followed by Stop Solution produces a yellow colored product which can be measured spectrophotometrically. The intensity of the color is directly proportional to the amount of bound Goat Anti-mouse IgG₁/HRP, which is proportional to the concentration of the anti-ovalbumin antibody.

$$\text{Absorbance} \propto [\text{Goat Anti-mouse IgG}_1/\text{HRP}] \propto [\text{Anti-ovalbumin antibody}]$$

A schematic of this process is shown in Figure 1, below.

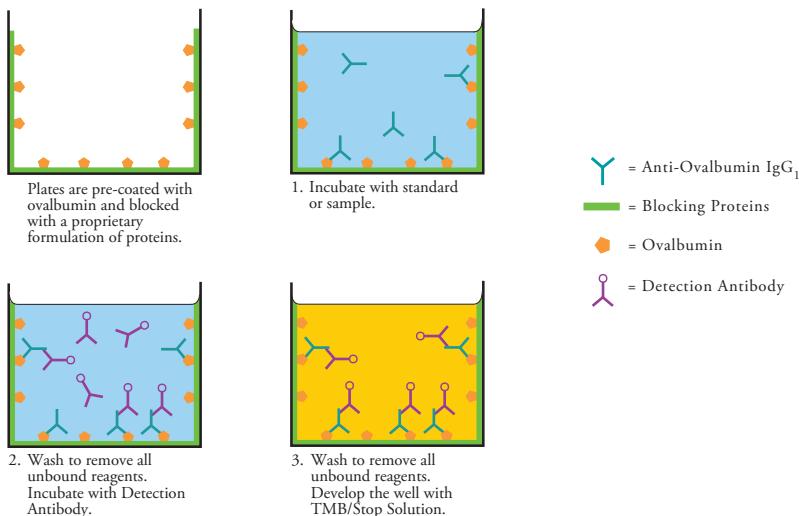


Figure 1. Schematic of the Immunometric EIA

PRE-ASSAY PREPARATION

Buffer Preparation

Store all diluted buffers at 4°C; they will be stable for about two months.

1. Assay Buffer Preparation

Dilute the contents of one vial of Immunoassay Buffer B Concentrate (10X) (Item No. 400054) with 90 ml of water. Be certain to rinse the vial to remove any salts that may have precipitated. *NOTE: It is normal for the concentrated buffer to contain crystalline salts after thawing. These will completely dissolve upon dilution with water.*

2. Wash Buffer Preparation

5 ml vial Wash Buffer Concentrate (400X) (Item No. 400062): Dilute to a total volume of 2 L with water and add 1 ml of Polysorbate 20 (Item No. 400035).

NOTE: Polysorbate 20 is a viscous liquid and cannot be measured by a regular pipette. A positive displacement pipette or a syringe should be used to deliver small quantities accurately.

Sample Preparation

Prior to use, it is recommended that serum or plasma samples from OVA/alum-immunized mice be diluted in Assay Buffer at least 1:2,000 in order to fall within the range of the standard curve (see Table 4 on page 16). In general, mouse serum or plasma (prepared using heparin or EDTA as the anticoagulant) can be used directly in the assay following dilution in Assay Buffer.

Preparation of Assay-Specific Reagents

Anti-Ovalbumin IgG₁ (mouse) EIA Standard

Reconstitute the lyophilized purified Anti-ovalbumin IgG₁ (mouse) EIA Standard (Item No. 400834) with 1.0 ml of Assay Buffer. Mix gently. The concentration of this solution (the bulk standard) is 200 ng/ml. The reconstituted standard is stable for two weeks at 4°C. Enough standard is provided to produce two duplicate-well standard curves for use on different days, if necessary.

To prepare the standard for use in the EIA: Obtain eight clean test tubes or plastic microfuge tubes and label them #1 through #8. Aliquot 250 µl of Assay Buffer into tubes #2-8. Transfer 500 µl of freshly prepared stock standard (200 ng/ml) to tube #1. Serially dilute the standard by removing 250 µl from tube #1 and placing into tube #2. Mix gently. Next, remove 250 µl from tube #2 and place into tube #3; mix gently. Repeat this process for tubes #4-8.

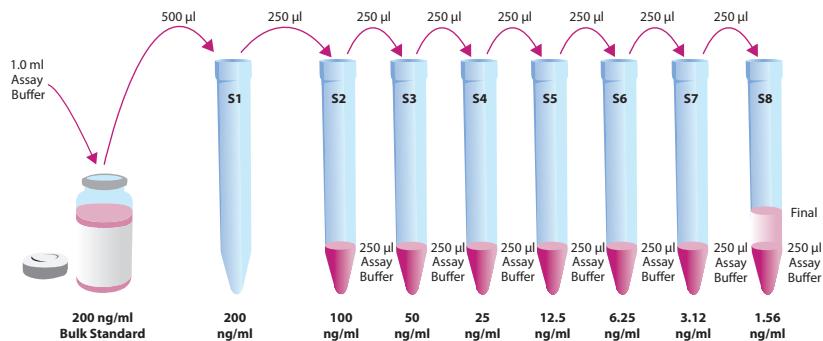


Figure 2. Preparation of the Anti-Ovalbumin IgG₁ (mouse) standards

Goat Anti-Mouse IgG₁ HRP Detection Antibody

This reagent is supplied as a concentrated (20X) stock solution of Goat anti-mouse IgG₁ polyclonal antibody conjugated to HRP. Just before use, prepare a Working Solution by adding 0.6 ml of the Goat Anti-mouse IgG₁ HRP Detection Antibody (Item No. 400830) to 11.4 ml Assay Buffer (12 ml total). In the event that two or more experiments are performed with this kit, sufficient stock solution has been provided to produce additional 12 ml of the Working Solution. Discard any leftover Working Solution.

Plate Set Up

The 96-well plate(s) included with this kit is supplied ready to use. It is not necessary to rinse the plate(s) prior to adding the reagents. *NOTE: If you do not need to use all of the strips at once, place the unused strips back in the plate packet and store according to the plate insert at 4°C. Be sure the packet is sealed with the desiccant inside.*

Each plate or set of strips must contain an eight point standard curve run in duplicate. *NOTE: Each assay must contain this minimum configuration in order to ensure accurate and reproducible results.* Each sample should be assayed at a minimum of two dilutions and each dilution should be assayed in duplicate. For statistical purposes, we recommend assaying samples in triplicate.

A suggested plate format is shown in Figure 3, on page 10. The user may vary the location and type of wells present as necessary for each particular experiment. The plate format provided below has been designed to allow for easy data analysis using a convenient spreadsheet offered by Cayman (see page 12, for more details). We suggest you record the contents of each well on the template sheet provided (see page 19).

	1	2	3	4	5	6	7	8	9	10	11	12
A	S1	S1	1	1	1	9	9	9	17	17	17	25
B	S2	S2	2	2	2	10	10	10	18	18	18	25
C	S3	S3	3	3	3	11	11	11	19	19	19	25
D	S4	S4	4	4	4	12	12	12	20	20	20	26
E	S5	S5	5	5	5	13	13	13	21	21	21	26
F	S6	S6	6	6	6	14	14	14	22	22	22	26
G	S7	S7	7	7	7	15	15	15	23	23	23	27
H	S8	S8	8	8	8	16	16	16	24	24	24	27

S1-S8 - Standards 1-8
1-27 - Samples

Figure 3. Sample plate format

Performing the Assay

Pipetting Hints

- Use different tips to pipette each reagent.
- Before pipetting each reagent, equilibrate the pipette tip in that reagent (*i.e.*, slowly fill the tip and gently expel the contents, repeat several times).
- Do not expose the pipette tip to the reagent(s) already in the well.

Addition of Standards and Samples and First Incubation

1. Add 100 μ l of the standards or diluted sample to the appropriate wells on the plate. Each sample should be assayed in duplicate, triplicate recommended.
2. Cover the plate with 96-Well Cover Sheet (Item No. 400012). Incubate for two hours at room temperature on an orbital shaker.

Addition of Goat Anti-Mouse IgG₁ HRP Detection Antibody and Second Incubation

1. Empty the wells and rinse four times with Wash Buffer. Each well should be completely filled with Wash Buffer during each wash. Invert the plate between wash steps to empty the fluid from the wells. After the last wash, gently tap the inverted plate on absorbent paper to remove the residual Wash Buffer.
2. Add 100 μ l of the Detection Antibody working solution to each well of the plate.
3. Cover the plate with plastic film and incubate for one hour at room temperature on an orbital shaker.

Development of the Plate

1. Empty the wells and rinse four times with Wash Buffer.
2. Add 100 μ l of TMB Substrate Solution (Item No. 400074) to each well of the plate.
3. Cover the plate with plastic film and incubate for 15 minutes at room temperature on an orbital shaker. Development of the blue color can be monitored at 650 nm. When the maximum standard (S1) optical density (O.D.) value reaches 0.5-0.6, Stop Solution should be added to the entire plate.
4. DO NOT WASH THE PLATE. Add 100 μ l of HRP Stop Solution (Item No. 10011355) to each well of the plate. Blue wells should turn yellow and colorless wells will remain colorless. *NOTE: The Stop Solution in this kit contains an acid. Wear appropriate protection and use caution when handling this solution.*

Reading the Plate

1. Wipe the bottom of the plate with a clean tissue to remove fingerprints, dirt, etc.
2. Read the plate at a wavelength of 450 nm.

ANALYSIS

Many plate readers come with data reduction software that plots data automatically. Alternatively a spreadsheet program can be used. *NOTE: Cayman has a computer spreadsheet available for data analysis. Please contact Technical Service or visit our website (www.caymanchem.com/analysis/immuno) to obtain a free copy of this convenient data analysis tool.*

Calculations

Plotting the Standard Curve and Determining the Sample Concentration

Using computer reduction software, plot absorbance (linear y-axis) for standards (S1-S8) versus concentration (linear x-axis) and fit the data with a quadratic equation. Using the equation of the line, calculate the concentration of anti-ovalbumin IgG₁ in each sample.

Performance Characteristics

Sample Data

The standard curve presented here is an example of the data typically produced with this kit; however, your results will not be identical to these. You **must** run a new standard curve. Do not use the data below to determine the values of your samples. Your results could differ substantially. Development of the plate for 15 minutes typically results in an absorbance of >1.0 O.D. units for the 200 ng/ml standard.

Anti-OVA IgG ₁ (ng/ml)	Absorbance	
200	2.520	2.422
100	1.481	1.424
50	0.857	0.828
25	0.494	0.473
12.5	0.292	0.293
6.25	0.179	0.182
3.12	0.120	0.122
1.56	0.108	0.099

Table 1. Typical results

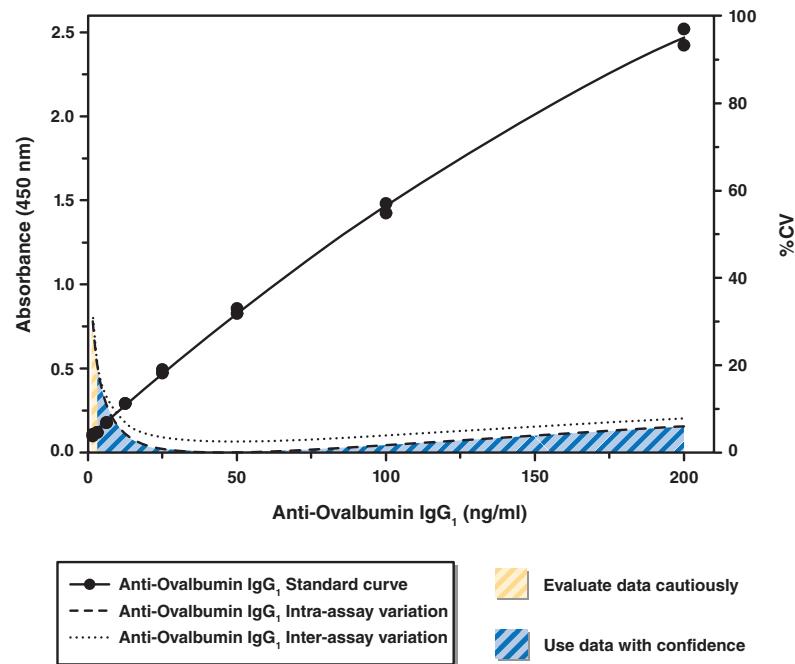


Figure 4. Typical standard curve

Precision:

The intra- and inter-assay CVs have been determined at multiple points on the standard curve. These data are summarized in the graph on page 13 and in the table below.

Anti-OVA IgG ₁ (ng/ml)	%CV* Intra-assay variation	%CV* Inter-assay variation
200	3.79	5.72
100	3.65	4.61
50	1.58	5.49
25	2.52	5.15
12.5	4.00	6.42
6.25	5.93	10.03
3.12	20.18	17.76
1.56	31.68†	35.44†

Table 2. Intra- and inter-assay variation

*%CV represents the variation in concentration (not absorbance) as determined using a reference standard curve.

†Outside of the recommended usable range of the assay.

Anti-OVA IgG ₁ (ng/ml)	Mean of O.D.	Standard Deviation (S.D.)	O.D. - (1.64 x S.D.)
200	2.875	0.055	2.784
100	1.788	0.048	1.709
50	1.034	0.014	1.011
25	0.604	0.012	0.584
12.5	0.348	0.010	0.331
6.25	0.210	0.007	0.198
3.12	0.129	0.008	0.114
1.56	0.112	0.008	0.125
0	0.012	0.011	0.030*

*O.D. + (1.64 x S.D.)

Table 3. Determination of LLOQ

The lower limit of quantitation (LLOQ) is defined as the lowest standard concentration in which O.D. - (1.64 x S.D.) is higher than the blank value of O.D. + (1.64 x S.D.). The LLOQ is 1.56 ng/ml.

Dilution Factor	Calculated Anti-OVA IgG ₁ concentration (mg/ml)				
	Plasma 1	Plasma 2	Plasma 3	Plasma 4	Plasma 5
500	Range	Range	Range	Range	Range
1,000	Range	Range	Range	Range	Range
2,000	0.425	Range	Range	Range	Range
4,000	0.475	Range	1.129	0.744	Range
8,000	0.469	1.371	1.058	0.734	1.396
16,000	0.481	1.318	1.079	0.779	1.543
32,000	0.461	1.303	1.147	0.766	1.386
64,000	0.411	1.343	1.121	0.795	1.440
Mean	0.454	1.334	1.107	0.769	1.441
S.D.	0.029	0.030	0.037	0.026	0.072

Table 4. Reproducibility of the assay over a wide dilution range

Plasma from five BALB/c female mice immunized with OVA/alum was diluted from 1:500 to 1:64,000 and the concentration of anti-OVA IgG₁ determined using Cayman's Anti-Ovalbumin IgG₁ (mouse) EIA Kit.

Range = outside standard curve range

RESOURCES

Troubleshooting

Problem	Possible Causes	Recommended Solutions
Erratic values; dispersion of duplicates	A. Trace organic contaminants in the water source B. Poor pipetting/technique	A. Replace activated carbon filter or change source of UltraPure water
Poor development (low signal) of standard curve	A. Plate required more development time B. Standard was diluted incorrectly C. Standard is degraded	

References

- Hogan, S.P., Mould, A., Kikutani, H., *et al.* Aeroallergen-induced eosinophilic inflammation, lung damage, and airways hyperreactivity in mice can occur independently of IL-4 and allergen-specific immunoglobulins. *J. Clin. Invest.* **99**(6), 1329-1339 (1997).
- Kennedy, J.D., Hatfield, C.A., Fidler, S.F., *et al.* Phenotypic characterization of T lymphocytes emigrating into lung tissue and the airway lumen after antigen inhalation in sensitized mice. *Am. J. Respir. Cell Mol. Biol.* **12**(6), 613-623 (1995).
- Saito, H., Howie, K., Wattie, J., *et al.* Allergen-induced murine upper airway inflammation: Local and systemic changes in murine experimental allergic rhinitis. *Immunology* **104**(2), 226-234 (2001).
- Sawada, K., Nagai, H., Basaki, Y., *et al.* The expression of murine cutaneous late phase reaction requires both IgE antibodies and CD4 T cells. *Clin. Exp. Allergy* **27**(2), 225-231 (1996).
- Pichavant, M., Goya, S., Hamelmann, E., *et al.* Animal models of airway sensitization. *Curr. Protoc. Immunol.* **79**, 15.18.1-15.18.19 (2007).
- Kung, T.T., Jones, H., Adams, G.K.I., *et al.* Characterization of a murine model of allergic pulmonary inflammation. *Int. Arch. Allergy Immunol.* **105**(1), 83-90 (1994).

NOTES

This document is copyrighted. All rights are reserved. This document may not, in whole or part, be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form without prior consent, in writing, from Cayman Chemical Company.

©07/07/2014, Cayman Chemical Company, Ann Arbor, MI, All rights reserved. Printed in U.S.A.