



# ADMA Xpress ELISA

*For the determination of ADMA in serum,  
citrate and EDTA plasma*

Valid from 2019-07-10

REF

KR7860



RUO



**Immundiagnostik AG**, Stubenwald-Allee 8a, 64625 Bensheim, Germany

Tel.: +49 6251 70190-0

Fax: + 49 6251 849430

e.mail: [info@immundiagnostik.com](mailto:info@immundiagnostik.com)

[www.immundiagnostik.com](http://www.immundiagnostik.com)

# Table of Contents

<b>1. INTENDED USE</b>	<b>2</b>
<b>2. MATERIAL SUPPLIED</b>	<b>2</b>
<b>3. MATERIAL REQUIRED BUT NOT SUPPLIED</b>	<b>2</b>
<b>4. STORAGE AND PREPARATION OF REAGENTS</b>	<b>3</b>
<b>5. STORAGE AND PREPARATION OF SAMPLES</b>	<b>4</b>
<b>6. ASSAY PROCEDURE</b>	<b>4</b>
<i>Principle of the test</i>	4
<i>Sample preparation procedure</i>	5
<i>Test procedure</i>	5
<b>7. RESULTS</b>	<b>6</b>
<b>8. LIMITATIONS</b>	<b>7</b>
<i>Analytical sensitivity</i>	8
<i>Biotin interference</i>	8
<b>9. QUALITY CONTROL</b>	<b>8</b>
<b>10. PERFORMANCE CHARACTERISTICS</b>	<b>8</b>
<i>Precision and reproducibility</i>	8
<b>11. PRECAUTIONS</b>	<b>9</b>
<b>12. TECHNICAL HINTS</b>	<b>9</b>
<b>13. GENERAL NOTES ON THE TEST AND TEST PROCEDURE</b>	<b>10</b>
<b>14. REFERENCES</b>	<b>10</b>
<i>General literature</i>	10
<i>Literature using Immundiagnostik ADMA Xpress ELISA</i>	11

## 1. INTENDED USE

This Immundiagnostik AG assay is intended for the quantitative determination of asymmetric dimethyl arginine (ADMA) in serum, citrate and EDTA plasma. For research use only. Not for use in diagnostic procedures.

## 2. MATERIAL SUPPLIED

Cat. No.	Label	Kit Components	Quantity
KR7860	PLATE	Microtiter plate, pre-coated	12 x 8 wells
KR7860	STD	Standards, ready-to-use (0, 0.1, 0.2, 0.4, 0.8, 2.0 $\mu$ M)	6 x 200 $\mu$ l
KR7860	CTRL 1	Control, ready-to-use (see specification for range)	1 x 200 $\mu$ l
KR7860	CTRL 2	Control, ready-to-use (see specification for range)	1 x 200 $\mu$ l
KR0006.C.100	WASHBUF A	Wash buffer concentrate, 10 x	2 x 100 ml
KR7860	REABUF	Reaction buffer, ready-to-use	1 x 22 ml
KR7860	CONJ	Conjugate, ready-to-use	1 x 12 ml
KR7860	DER	Derivatisation reagent, lyophilised	1 vial
KR0008.04	DMSO	Dimethylsulfoxide (DMSO)	1 x 4 ml
KR7860	CODIL	Dilution buffer after derivatization, ready-to-use	1 x 18 ml
KR0002.15	SUB	Substrate (tetramethylbenzidine), ready-to-use	1 x 15 ml
KR0003.15	STOP	Stop solution, ready-to-use	1 x 15 ml

For reorders of single components, use the catalogue number followed by the label as product number.

## 3. MATERIAL REQUIRED BUT NOT SUPPLIED

- Ultrapure water\*
- Calibrated precision pipets and 10-1000  $\mu$ l single-use tips
- Foil to cover the microtiter plate
- Horizontal microtiter plate shaker
- Multi-channel pipets or repeater pipets

- Vortex
- Standard single-use laboratory glass or plastic vials, cups, etc.
- Microtiter plate reader (required filters see chapter 6)

\* Immundiagnostik AG recommends the use of ultrapure water (water type 1; ISO 3696), which is free of undissolved and colloidal ions and organic molecules (free of particles > 0.2 µm) with an electrical conductivity of 0.055 µS/cm at 25 °C (≥18.2 MΩ cm).

## 4. STORAGE AND PREPARATION OF REAGENTS

- To run the assay more than once, ensure that reagents are stored at the conditions stated on the label.
- **Preparation of the wash buffer:** The **wash buffer concentrate (WASHBUF A)** has to be diluted with ultrapure water **1:10** before use (100 ml WASHBUF A + 900 ml ultrapure water), mix well. Crystals could occur due to high salt concentration in the concentrate. Before dilution, the crystals have to be redissolved at room temperature or in a water bath at 37 °C. The **WASHBUF A** is stable at **2-8 °C** until the expiry date stated on the label. **Wash buffer** (1:10 diluted WASHBUF A) can be stored in a closed flask at **2-8 °C for 1 month**.
- Store **standards and controls (STD/CTRL)** frozen at **-20 °C**. They are stable at -20 °C until the expiry date stated on the label. Thaw before use in the test and mix well. Re-freeze standards and controls after use.
- The **reaction buffer (REABUF)** is stable at **2-8 °C** until the expiry date stated on the label. Bring to room temperature before use and dissolve any occurring crystals.
- **DMSO** crystallises at 2-8 °C. Before use, bring to room temperature to dissolve the crystals.
- The **lyophilised derivatisation reagent (DER)** is stable at **2-8 °C** until the expiry date stated on the label. Bring to room temperature before opening and reconstitute the content of the vial with **3 ml DMSO**. Mix thoroughly with a vortex-mixer and allow to dissolve for 10 minutes. **The derivatisation reagent** (reconstituted DER) **can be stored at 2-8 °C for 2 months**. Bring to room temperature before reuse. Please note: DMSO attacks all plastics but not polypropylene products and laboratory glass.
- All other test reagents are ready-to-use. Test reagents are stable until the ring **all reagents and samples to room temperature** (15-30 °C) and mix well. expiry date (see label) when stored at **2-8 °C**.

## 5. STORAGE AND PREPARATION OF SAMPLES

### Serum, citrate and EDTA plasma

- Freshly collected serum or plasma can be stored for 3 days at room temperature (15-30 °C) or at 2-8 °C. For longer storage keep frozen at -20 °C.
- Lipemic or hemolytic samples may give erroneous results and should not be used for analysis.
- EDTA plasma and serum samples are used **undiluted**.  
If sample dilution is required, use STD1 (zero-standard) as diluent.
- For sample preparation, a derivatisation reagent for derivatisation of ADMA is added (details are given in the sample preparation procedure).

## 6. ASSAY PROCEDURE

### *Principle of the test*

This ELISA is designed for the quantitative determination of ADMA. This assay is based on the method of competitive enzyme linked immunoassays.

The sample preparation includes the addition of a derivatisation reagent for ADMA derivatisation, and a reaction buffer is added containing ADMA-derivative (tracer). Afterwards, the treated samples are incubated in wells of a microtiter plate coated with a polyclonal antibody against ADMA-derivative. During the incubation period the target ADMA in the sample competes with the tracer for the binding of the polyclonal antibodies, immobilised on the wall of the microtiter wells.

During the second incubation step a peroxidase conjugate is added to each microtiter well to detect the tracer. After washing away the unbound components, tetramethylbenzidine (TMB) is added as a peroxidase substrate. Finally, the enzymatic reaction is terminated by an acidic stop solution. The colour changes from blue to yellow, and the absorbance is measured in a photometer at 450 nm. The intensity of the yellow colour is inverse proportional to the ADMA concentration in the sample; this means, high ADMA concentration in the sample reduces the concentration of antibody-bound tracer and lowers the photometric signal. A dose response curve of the absorbance unit (optical density, OD at 450 nm) vs. concentration is generated, using the values obtained from the standards. ADMA, present in the samples, is determined directly from this curve.

### *Sample preparation procedure*

Bring **all reagents and samples to room temperature** (15-30 °C) and mix well.

Derivatisation of standards, controls and samples is carried out in single analysis in vials (e.g. 1.5 ml polypropylene vials).

We recommend preparing one derivatisation per standard, control and sample and transferring it in duplicate determinations into the wells of the microtiter plate.

1.	Add <b>25 µl standard (STD)/control (CTRL)/sample</b> into the corresponding vials.
2.	Add <b>200 µl reaction buffer (REABUF)</b> into each vial (STD, CTRL, sample).
3.	Add <b>25 µl derivatisation reagent</b> into each vial (STD, CTRL, sample) and <b>mix thoroughly</b> by repeated inversion or several seconds on a vortex mixer. Incubate for <b>30 min at room temperature</b> (15-30 °C) on a <b>horizontal shaker</b> .

2 x 50 µl of the derivatised standards/controls/samples are used in the ELISA as duplicates.

### *Test procedure*

Mark the positions of standards/controls/samples in duplicate on a protocol sheet.

Take as many microtiter strips as needed from the kit. Store unused strips together with the desiccant bag in the closed aluminium packaging at 2-8 °C. Strips are stable until the expiry date stated on the label.

4.	<b>Before use</b> , wash the wells <b>5 times</b> with <b>250 µl wash buffer</b> . After the final washing step, remove residual wash buffer by firmly tapping the plate on absorbent paper.
5.	Add <b>150 µl dilution buffer (CODIL)</b> into each well of the microtiter plate.
6.	For the analysis in duplicate take <b>2 x 50 µl</b> of the <b>derivatised standards/controls/samples</b> out of the vials and add into the respective wells of the microtiter plate.
7.	Cover the strips and incubate for <b>2 hours at room temperature</b> (15-30 °C) on a <b>horizontal shaker</b> .

8.	Discard the content of each well and wash <b>5 times</b> with <b>250 µl wash buffer</b> . After the final washing step, remove residual wash buffer by firmly tapping the plate on absorbent paper.
9.	Add <b>100 µl conjugate</b> (CONJ) into each well.
10.	Cover the strips and incubate for <b>30 minutes</b> at room temperature (15-30 °C) on a <b>horizontal shaker</b> .
11.	Discard the content of each well and wash <b>5 times</b> with <b>250 µl wash buffer</b> . After the final washing step, remove residual wash buffer by firmly tapping the plate on absorbent paper.
12.	Add <b>100 µl substrate</b> (SUB) into each well.
13.	Incubate for <b>8-12 min*</b> at room temperature (15-30 °C) in the <b>dark</b> .
14.	Add <b>100 µl stop solution</b> (STOP) into each well and mix well.
15.	Determine <b>absorption immediately</b> with an ELISA reader at <b>450 nm</b> against 620 nm (or 690 nm) as a reference. If no reference wavelength is available, read only at 450 nm. If the extinction of the highest standard exceeds the range of the photometer, absorption must be measured immediately at <b>405 nm</b> against 620 nm (690 nm) as a reference.

\* The intensity of the color change is temperature sensitive. We recommend observing the color change and stopping the reaction upon good differentiation.

For automated ELISA processors, the given protocol may need to be adjusted according to the specific features of the respective automated platform. For further details please contact your supplier or Immundiagnostik AG.

## 7. RESULTS

The following algorithms can be used alternatively to calculate the results. We recommend using the 4 parameter algorithm.

### 1. 4 parameter algorithm

It is recommended to use a linear ordinate for optical density and a logarithmic abscissa for concentration. When using a logarithmic abscissa, the zero standard must be specified with a value less than 1 (e.g. 0.001).

## 2. Point-to-point calculation

We recommend a linear ordinate for optical density and a linear abscissa for concentration.

## 3. Spline algorithm


We recommend a linear ordinate for optical density and a linear abscissa for concentration.

The plausibility of the duplicate values should be examined before the automatic evaluation of the results. If this option is not available with the program used, the duplicate values should be evaluated manually.

### Serum, citrate and EDTA plasma

**No factor** is required.

In the following, an example of a standard curve is given. Do not use it for the calculation of your results.

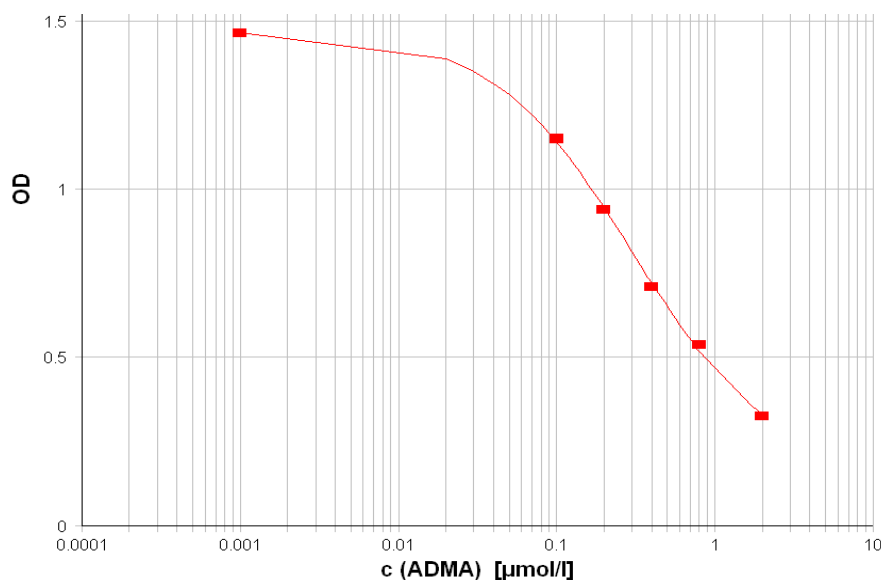

## 8. LIMITATIONS

Samples with concentrations above the measurement range (see definition below) can be diluted with Standard 1 (zero-standard) and re-assayed. Please consider this dilution factor when calculating the results.

Samples with concentrations lower than the measurement range (see definition below) cannot be clearly quantified.

The upper limit of the measurement range can be calculated as:

*highest concentration of the standard curve × sample dilution factor to be used*



The lower limit of the measurement range can be calculated as:

*Analytical sensitivity* × *sample dilution factor to be used*

### *Analytical sensitivity*

The zero-standard (STD 1) was measured 46 times. The detection limit was set as  $B_0 - 2 \text{ SD}$  and estimated to be 0.04  $\mu\text{mol/l}$ .

### *Biotin interference*

Samples containing a biotin concentration of  $\leq 1200 \text{ ng/ml}$  show a change of the results of  $< 25 \%$ . Higher concentrations of biotin can lead to falsely low results. Subjects taking  $> 5 \text{ mg}$  biotin per day should wait at least 24 hours after taking biotin to have their samples collected. Results of subjects taking biotin supplements or receiving a high-dose biotin therapy should generally be interpreted along with the total health picture.

## 9. QUALITY CONTROL

Immundiagnostik AG recommends the use of external controls for internal quality control, if possible.

Control samples should be analysed with each run. Results, generated from the analysis of control samples, should be evaluated for acceptability using appropriate statistical methods. The results for the samples may not be valid if within the same assay one or more values of the quality control samples are outside of the acceptable limits.

We recommend each laboratory to establish its own reference range.

## 10. PERFORMANCE CHARACTERISTICS

### *Precision and reproducibility*

#### **Intra-assay (n = 12)**

<b>Sample</b>	<b>ADMA [<math>\mu\text{mol/l}</math>]</b>	<b>CV [%]</b>
1	0.19	7.9
2	0.48	5.8

**Inter-assay (n = 6)**

Sample	ADMA [ $\mu\text{mol/l}$ ]	CV [%]
1	0.19	10.8
2	0.47	7.6

**11. PRECAUTIONS**

- All reagents in the kit package are for research use only.
- Human materials used in kit components were tested and found to be negative for HIV, Hepatitis B and Hepatitis C. However, for safety reasons, all kit components should be treated as potentially infectious.
- Kit reagents contain thimerosal or ProClin as bactericides. Thimerosal and ProClin are toxic. Substrates for the enzymatic colour reactions are toxic and carcinogenic. Avoid contact with skin or mucous membranes.
- The stop solution consists of diluted sulfuric acid, a strong acid. Although diluted, it still must be handled with care. It can cause burns and should be handled with gloves, eye protection, and appropriate protective clothing. Any spill should be wiped up immediately with copious quantities of water. Do not breathe vapour and avoid inhalation.

**12. TECHNICAL HINTS**

- Do not interchange different lot numbers of any kit component within the same assay. Furthermore, we recommend not assembling wells of different microtiter plates for analysis, even if they are of the same batch.
- Control samples should be analysed with each run.
- Reagents should not be used beyond the expiration date stated on the kit label.
- Substrate solution should remain colourless until use.
- To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
- Avoid foaming when mixing reagents.
- Do not mix plugs and caps from different reagents.
- The assay should always be performed according to the enclosed manual.

### 13. GENERAL NOTES ON THE TEST AND TEST PROCEDURE

- The guidelines for laboratories should be followed.
- Incubation time, incubation temperature and pipetting volumes of the components are defined by the producer. Any variation of the test procedure, which is not coordinated with the producer, may influence the results of the test. Immundiagnostik AG can therefore not be held responsible for any damage resulting from incorrect use.
- Warranty claims and complaints regarding deficiencies must be logged within 14 days after receipt of the product. The product should be sent to Immundiagnostik AG along with a written complaint.

### 14. REFERENCES

#### *General literature*












1. Böger RH, Bode-Böger SM, Szuba A, Tangphao O, Tsao PS, Chan JR, Blaschke TF, Cooke JP. Asymmetric dimethylarginine: a novel risk factor for endothelial dysfunction. Its role in hypercholesterolemia. *Circulation* 1998; **98**: 1842 – 1847
2. Böger RH. The emerging role of asymmetric dimethylarginine as a novel cardiovascular risk factor. *Cardiovasc. Res.* 2003; **59**: 824-833
3. Kielstein JT, Böger RH, Bode-Böger SM, et al. Asymmetric dimethylarginine plasma concentrations differ in patients with end-stage renal disease: Relationship to treatment method and atherosclerotic disease. *J. Am. Soc. Nephrol.* 1999; **10**: 594 – 600
4. Lu TM, Ding YA, Lin SJ, Lee WS, Tai HC. Plasma levels of asymmetrical dimethylarginine and adverse cardiovascular events after percutaneous coronary intervention. *Eur Heart J.* 2003; **24**: 1912-1919
5. Nijveldt RJ, Teerlink T, Van der Hoven B, Siroen MP, Kuik DJ, Rauwerda JA, van Leeuwen PA. Asymmetrical dimethylarginine (ADMA) in critically ill patients: high plasma ADMA concentration is an independent risk factor of ICU mortality. *Clin. Nutr.* 2003; **22**: 23-30
6. Savvidou MD, Hingorani AD, Tsikas D, Frolich JC, Vallance P, Nicolaides KH. Endothelial dysfunction and raised plasma concentrations of asymmetric dimethylarginine in pregnant women who subsequently develop pre-eclampsia. *Lancet* 2003; **361**: 1511-1517
7. Stühlinger M, Abbasi F, Chu JW, Lamendola C, McLaughlin TL, Cooke JP, Reaven GM, Tsao PS. Relationship between insulin resistance and an endogenous nitric oxide synthase inhibitor. *J. Am. Med. Assoc.* 2002; **287**: 1420-1426

8. Vallance P, Leone A, Calver A, Collier J, Moncada S. Accumulation of an endogenous inhibitor of NO synthesis in chronic renal failure. *Lancet* 1992; **339**: 572 – 575
9. Zoccali C, Bode-Böger SM, Mallamaci F, Benedetto FA, Tripepi G, Malatino L, Cataliotti A, Bellanuova I, Fermo I, Frölich JC, Böger RH. Asymmetric dimethylarginine (ADMA): An endogenous inhibitor of nitric oxide synthase predicts mortality in end-stage renal disease (ESRD). *Lancet* 2001; **358**: 2113-2117

### Literature using Immundiagnostik ADMA Xpress ELISA

10. Dzikowska-Diduch O, Kostrubiec M, Domienik-Karłowicz J, Wyzgal A, Labyk A, Radochonska J, Gorska E, Demkow U, Pruszczyk P. Endothelial Dysfunction in Patients with History of Pulmonary Embolism. *Eur Heart J.* 2010, **34** (suppl 1): 202–203
11. Watarai R, Suzuki K, Ichino N, Osakabe K, Sugimoto K, Yamada H, Hamajima T, Hamajima N, Inoue T. Association between serum levels of carotenoids and serum asymmetric dimethylarginine levels in Japanese subjects. *Epidemiol* 2014, **24** (3): 250-257

#### Used symbols:

	Temperature limitation		Catalogue Number
	For research use only		To be used with
	Manufacturer		Contains sufficient for <n> tests
	Lot number		Use by
	Attention		Consult instructions for use
	Consult specification data sheet		

