



Magnetic Luminex® Performance Assay Human CXCL8/IL-8 High Sensitivity Kit

Catalog Number: LHSCM208


Pack Size: 100 Tests

SPECIFICATIONS & USE

- Recommended Sample Types**
- Serum, EDTA plasma, and heparin plasma.
- Microparticle Region**
- Region-26
- Components**
- Microparticle Concentrate (Part 894495) is supplied as a 50X concentrated stock (0.075 mL) with preservatives.
 - Biotin-Antibody Concentrate (Part 894052) is supplied as a 100X concentrated stock solution (0.075 mL) with preservatives.
- Other Supplies Required**
- Magnetic Luminex Performance Assay Human High Sensitivity Cytokine Base Kit A (Catalog Number LHSCM000).
- Storage**
- Store the unopened kit at 2-8 °C. Do not use past the expiration date on the label.
 - **Avoid freezing microparticles.**
 - **Protect microparticles from light.**
- Instructions for Use**
- Refer to the Base Kit insert for the Magnetic Luminex Performance Assay procedure.

TYPICAL DATA

This human IL-8 standard curve is provided only for demonstration. A standard curve must be generated each time an assay is run, utilizing values from the Standard Value Card included in the Base Kit.

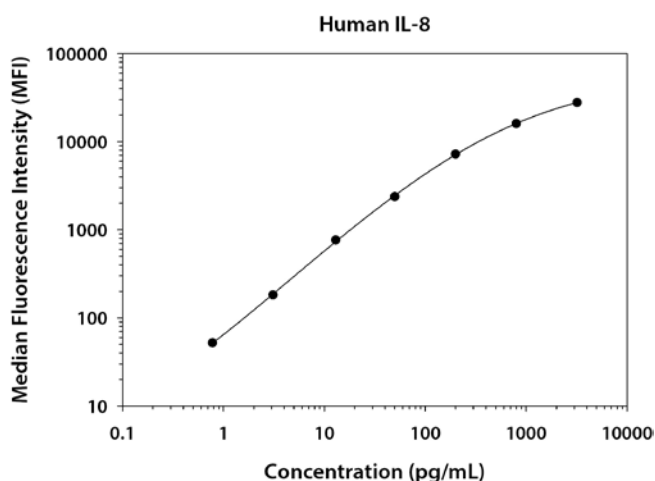

Standard	pg/mL	MFI	Average	Corrected
Blank	0	41 43	42	—
1	3200	27,787 27,982	27,885	27,843
2	800	15,817 16,391	16,104	16,062
3	200	7237 7282	7260	7218
4	50	2405 2441	2423	2381
5	13	807 807	807	765
6	3.1	222 226	224	182
7	0.78	94 94	94	52

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

R&D Systems, Inc.
1-800-343-7475

PRECISION

Intra-assay Precision (precision within an assay)

Three samples of known concentration were tested twenty times on one plate to assess precision within an assay.

Inter-assay Precision (precision between assays)

Three samples of known concentration were tested in separate assays to assess precision between assays.

	Intra-assay Precision			Inter-assay Precision		
Sample	1	2	3	1	2	3
n	20	20	20	60	60	60
Mean (pg/mL)	7.2	48	874	6.8	46	981
Standard Deviation	0.3	2.1	99	0.7	3.8	154
% CV	4.2	4.4	11.3	10.3	8.3	15.7

RECOVERY & LINEARITY

Samples were spiked with human IL-8 and evaluated for recovery and were serially diluted to evaluate assay linearity.

Recovery			Linearity				
Sample Type	Average % Recovery	Range (%)			Serum	EDTA Plasma	Heparin Plasma
Serum	86	60-131	1:2	Average % of Expected	115	101	112
				Range (%)	95-126	77-129	99-119
EDTA plasma	83	67-102	1:4	Average % of Expected	126	101	112
				Range (%)	101-143	70-126	102-123
Heparin plasma	91	63-97	1:8	Average % of Expected	123	101	121
				Range (%)	113-133	72-127	109-132

SENSITIVITY

All data were collected with assays run as a multiplex.

Data obtained with polystyrene and magnetic beads were equivalent.

Twenty-eight assays were evaluated, and the minimum detectable dose (MDD) of human IL-8 ranged from 0.02-0.07 pg/mL. The mean MDD was 0.04 pg/mL.

The MDD was determined by adding two standard deviations to the MFI of twenty zero standard replicates and calculating the corresponding concentration.

CORRELATION

This assay has been correlated to the Quantikine® ELISA Kit with a slope of 0.9-1.1 and an R² value greater than 0.9.

SPECIFICITY

Note: Refer to the base kit insert for a complete list of analytes tested for cross-reactivity and interference.

This assay recognizes natural and recombinant human IL-8.

Recombinant feline IL-8 interferes at concentrations ≥ 1.562 ng/mL.

TECHNICAL HINTS

- Protect the microparticles and streptavidin-PE from light at all times.
- Refer to the appropriate Base Kit Standard Value Card for reconstitution volume and values of the reconstituted standard.
- Diluted microparticles cannot be stored. Make a fresh dilution of microparticles each time the assay is run.
- The use of a magnetic device made to accommodate a microplate is necessary for washing.
- Discrepancies may exist in values obtained for the same analyte utilizing different technologies.

Luminex Performance Assays afford the user the benefit of multianalyte analysis of cytokines in a complex sample. A single, multipurpose diluent is used to optimize recovery, linearity, and reproducibility. Such a multipurpose, single diluent may not optimize any single analyte to the same degree that a unique diluent selected for analysis of that analyte can optimize conditions. Therefore, some performance characteristics may be more variable than those for assays designed specifically for single analyte analysis.

All trademarks and registered trademarks are the property of their respective owners.