

Human Total 25-OH Vitamin D IVD ELISA

GENERAL INFORMATION

- A. Proprietary name: Human Total 25-OH Vitamin D IVD ELISA Kit
- B. Catalog Number: RDKAP1971, 96 tests
- C. Manufactured for: R&D Systems, a Bio-Techne brand

This package insert must be read in its entirety before using this product.

IVD For *In Vitro* Diagnostic use.

TABLE OF CONTENTS

SECTION	PAGE
I. INTENDED USE	1
II. CLINICAL BACKGROUND	1
III. PRINCIPLES OF THE METHOD.....	1
IV. REAGENTS PROVIDED.....	2
V. PRECAUTIONS AND WARNINGS	3
VI. STORAGE AND EXPIRATION DATING OF REAGENTS.....	3
VII. SUPPLIES NOT PROVIDED.....	3
VIII. REAGENT PREPARATION	4
IX. SPECIMEN COLLECTION AND PREPARATION	5
X. PROCEDURE.....	5
XI. CALCULATION OF RESULTS.....	6
XII. PERFORMANCE AND LIMITATIONS.....	7
XIII. INTERNAL QUALITY CONTROL	12
XIV. EXPECTED VALUES	12
XV. BIBLIOGRAPHY	13
XVI. SUMMARY OF THE PROTOCOL.....	14

DISTRIBUTED BY:

USA & Canada | Bio-Techne Corp.

614 McKinley Place NE, Minneapolis, MN 55413, USA
TEL: (800) 343-7475 (612) 379-2956 FAX: (612) 656-4400
E-MAIL: info@bio-techne.com

UK & Europe | Bio-Techne EMEA

19 Barton Lane, Abingdon Science Park, Abingdon OX14 3NB, UK
TEL: +44 (0)1235 529449 FAX: +44 (0)1235 533420
E-MAIL: info@bio-techne.com

China | Bio-Techne China

24A1 Hua Min Empire Plaza, 726 West Yan An Road, Shanghai PRC 200050
TEL: +86 (21) 52380373 FAX: +86 (21) 52371001
E-MAIL: info@bio-techne.com

I. INTENDED USE

Immunoenzymetric assay for the in vitro quantitative measurement of 25-hydroxyvitamin D2 and D3 (25-OH-D2 and 25-OH-D3) in serum.

II. CLINICAL BACKGROUND

Vitamin D is the generic term used to designate Vitamin D2 or ergocalciferol and Vitamin D3 or cholecalciferol. Humans naturally produce Vitamin D3 when the skin is exposed to ultraviolet sun rays. In the liver mainly, Vitamin D3 is metabolized into 25-hydroxyvitamin D3 (25-OH-D3) which is the main form of Vitamin D circulating in the body. 25-OH-D3 is a precursor for other Vitamin D metabolites and has also a limited activity by itself. The most active derivative is 1, 25-hydroxyvitamin D3, produced in the kidney (or placenta) by 1-hydroxylation of 25-OH-D3. 25-OH Vitamin D stimulates the intestinal absorption of both calcium and phosphorus and also bone resorption and mineralization. 25-OH Vitamin D might also be active in other tissues responsible for calcium transport for example, placenta, kidney, mammary gland and endocrine gland, parathyroid glands, and beta cells. Vitamin D3 and Vitamin D2 are also available by ingestion through food or dietary supplementation. As Vitamin D2 is metabolized in a similar way to Vitamin D3, both contribute to the overall Vitamin D status of an individual. It is the reason why it is very important to measure both forms of 25-OH Vitamin D equally for a correct diagnosis of Vitamin D deficiency, insufficiency or intoxication. Vitamin D deficiency is an important risk factor for rickets, osteomalacia, senile osteoporosis, and cancer and pregnancy outcomes. The measurement of both 25-OH Vitamin D forms is also required to determine the cause of abnormal serum calcium concentrations in patients. Vitamin D intoxication has been shown to cause kidney and tissue damage.

III. PRINCIPLES OF THE METHOD

The Human Total 25-OH Vitamin D IVD ELISA is a solid phase Enzyme Linked Immunosorbent Assay performed on microplates. During the first two hour incubation step, at room temperature, total 25-OH Vitamin D (D2 and D3) present in calibrators, controls and samples is dissociated from binding serum proteins to fix on binding sites of a specific monoclonal antibody. After one washing step, a fixed amount of 25-OH Vitamin D-labeled with biotin in presence of horseradish peroxidase (HRP), competes with labeled 25-OH Vitamin D2 and 25-OH Vitamin D3 present on the binding sites of the specific monoclonal antibody. After a 30 minute incubation at room temperature, the microplate is washed to stop the competition reaction. The Chromogenic solution TMB is added and incubated for 15 minutes. The reaction is stopped with the addition of Stop solution and the microplate is then read at the appropriate wavelength. The amount of substrate turnover is determined colorimetrically by measuring the absorbance, which is inversely proportional to the total 25-OH Vitamin D (D2 and D3) concentration. A calibration curve is plotted and the total 25-OH Vitamin D (D2 and D3) concentrations of the samples are determined by dose interpolation from the calibration curve.

IV. REAGENTS PROVIDED

REAGENTS	96 TEST KIT	COLOR CODE	RECONSTITUTION			
 Microplate (96 breakable wells) with anti 25-OH Vitamin D2 and D3 (monoclonal antibodies)	96 wells	blue	Ready for use			
<table border="1" data-bbox="138 367 300 420"> <tr> <td>CAL</td> <td>0</td> </tr> </table> Calibrator 0: biological matrix with gentamycin and proclin	CAL	0	1 vial lyophilized	yellow	Add 2 mL distilled water	
CAL	0					
<table border="1" data-bbox="138 525 300 577"> <tr> <td>CAL</td> <td>N</td> </tr> </table> Calibrators 1-5 (see exact values on vial labels) in horse serum with gentamycin and proclin	CAL	N	5 vials lyophilized	yellow	Add 1 mL distilled water	
CAL	N					
<table border="1" data-bbox="138 682 381 735"> <tr> <td>CONTROL</td> <td>N</td> </tr> </table> Controls N = 2 in human serum with proclin	CONTROL	N	2 vials lyophilized	silver	Add 1 mL distilled water	
CONTROL	N					
<table border="1" data-bbox="138 798 332 850"> <tr> <td>INC</td> <td>BUF</td> </tr> </table> Incubation Buffer with casein and proclin	INC	BUF	1 vial 20 mL	green	Ready for use	
INC	BUF					
<table border="1" data-bbox="138 913 349 966"> <tr> <td>CONJ</td> <td>CONC</td> </tr> </table> 25-OH Vitamin D Concentrated Conjugate	CONJ	CONC	1 vial 0.3 mL	blue	Dilute 100X with Conjugate Buffer	
CONJ	CONC					
<table border="1" data-bbox="138 1029 332 1081"> <tr> <td>CONJ</td> <td>BUF</td> </tr> </table> Conjugate Buffer with casein and proclin	CONJ	BUF	1 vial 30 mL	red	Ready for use	
CONJ	BUF					
<table border="1" data-bbox="138 1144 397 1197"> <tr> <td>HRP</td> <td>CONC</td> </tr> </table> Concentrated HRP	HRP	CONC	1 vial 0.2 mL	yellow	Dilute 200X with Conjugate Buffer	
HRP	CONC					
<table border="1" data-bbox="138 1260 446 1312"> <tr> <td>WASH</td> <td>SOLN</td> <td>CONC</td> </tr> </table> Wash solution (TRIS-HCl)	WASH	SOLN	CONC	1 vial 10 mL	brown	Dilute 200X with distilled water (use a magnetic stirrer)
WASH	SOLN	CONC				
<table border="1" data-bbox="138 1375 397 1428"> <tr> <td>CHROM</td> <td>TMB</td> </tr> </table> Chromogenic solution TMB (Tetramethylbenzidine)	CHROM	TMB	1 vial 12 mL	orange	Ready for use	
CHROM	TMB					
<table border="1" data-bbox="138 1491 349 1543"> <tr> <td>STOP</td> <td>SOLN</td> </tr> </table> Stop solution HCl 1M	STOP	SOLN	1 vial 12 mL	none	Ready for use	
STOP	SOLN					

Note: Use Calibrator 0 for dilution of samples with values above the highest calibrator. No international reference material is available.

V. PRECAUTIONS AND WARNINGS

Safety

For *in vitro* diagnostic use only.

The human blood components included in this kit have been tested by European approved and/or FDA approved methods and found negative for HBsAg, anti-HCV, anti-HIV-1 and 2. No known method can offer complete assurance that human blood derivatives will not transmit hepatitis, AIDS or other infections. Therefore, handling of reagents and serum specimens should be in accordance with local safety procedures.

All animal products and derivatives have been collected from healthy animals. Bovine components originate from countries where BSE has not been reported. Nevertheless, components containing animal substances should be treated as potentially infectious.

Avoid any skin contact with all reagents, Stop solution contains HCl. In case of contact, wash thoroughly with water.

Do not smoke, drink, eat or apply cosmetics in the working area. Do not pipette by mouth. Use protective clothing and disposable gloves.

VI. STORAGE AND EXPIRATION DATING OF REAGENTS

- Before opening or reconstitution, all kit components are stable until the expiry date, indicated on the label, if kept at 2-8 °C.
- After reconstitution, calibrators and controls are stable for eight weeks at 2-8 °C. For longer storage periods, aliquots should be made and kept at ≤ -20 °C for a maximum of 4 months. Avoid subsequent freeze-thaw cycles.
- Freshly prepared Working Wash solution should be used on the same day.
- Alterations in physical appearance of kit reagents may indicate instability or deterioration.

VII. SUPPLIES NOT PROVIDED

The following materials are required but not provided in the kit:

1. Distilled water
2. Pipettes for delivery of: 50 μ L, 150 μ L, 200 μ L and 1 mL (the use of accurate pipettes with disposable plastic tips is recommended)
3. Vortex mixer
4. Magnetic stirrer
5. Plate shaker (300 to 700 rpm)
6. Washer for microplates
7. Microplate reader capable of reading at 450 nm and 630 or 650 nm (bichromatic reading)

VIII. REAGENT PREPARATION

A. Calibrator 0: Reconstitute the Calibrator 0 with 2 mL distilled water.

B. Calibrators 1-5: Reconstitute the Calibrators 1-5 with 1 mL distilled water.

C. Controls: Reconstitute the Controls with 1 mL distilled water.

D. Working HRP conjugate solution:

The Working HRP conjugate solution should be prepared during the incubation and a minimum of 1 hour 45 minutes before its use (cf XI.B.5).

Prepare an adequate volume of Working HRP conjugate solution by mixing Concentrated Conjugate, Concentrated HRP and Conjugate Buffer according to the number of used strips, as indicated in the table below:

Example: for 6 strips (48 wells), add 100 µL of Concentrated Conjugate and 50 µL of Concentrated HRP to 10 mL of Conjugate Buffer.

Use a vortex to homogenize.

Until its use keep the Working HRP conjugate solution at room temperature and avoid direct sunlight or use a brown glass vial for its preparation.

The preparation of Working HRP conjugate solution is not stable and must be discarded if not used.

Number of strips	Volume of Concentrated Conjugate (µL)	Volume of Concentrate HRP (µL)	Volume of Conjugate Buffer (mL)
1	30	15	3
2	50	25	5
3	60	30	6
4	80	40	8
5	90	45	9
6	100	50	10
7	120	60	12
8	140	70	14
9	160	80	16
10	180	90	18
11	200	100	20
12	220	110	22

E. Working Wash solution: Prepare an adequate volume of Working Wash solution by adding 199 volumes of distilled water to 1 volume of Wash solution (200X). Use a magnetic stirrer to homogenize. Discard unused Working Wash solution at the end of the day.

IX. SPECIMEN COLLECTION AND PREPARATION

- This kit is suitable for serum samples.
- Serum samples must be kept at 2-8 °C.
- If the test is not run within 24 hours, **sampling and storage at ≤ -20 °C is recommended.**
- Avoid subsequent freeze-thaw cycles.

X. PROCEDURE

A. Handling notes

- Do not use the kit or components beyond expiry date.
- Do not mix materials from different kit lots.
- Bring all the reagents to room temperature prior to use.
- Thoroughly mix all reagents and samples by gentle agitation or swirling.
- Perform calibrators, controls and samples in duplicate. Vertical alignment is recommended.
- Use a clean plastic container to prepare the Working Wash solution.
- In order to avoid cross-contamination, use a clean disposable pipette tip for the addition of each reagent and sample.
- For the dispensing of Chromogenic solution and Stop solution avoid pipettes with metal parts.
- High precision pipettes or automated pipetting equipment will improve the precision.
- Respect the incubation times.
- To avoid drift, the time between pipetting of the first calibrator and the last sample must be limited to the time mentioned in section XIII paragraph G (Time delay).
- Prepare a calibration curve for each run, do not use data from previous runs.
- Dispense the Chromogenic solution within 15 minutes following the washing of the microplate.
- During incubation with Chromogenic solution, avoid direct sunlight on the microplate.

B. Procedure

1. Select the required number of strips for the run. The unused strips should be resealed in the bag with a desiccant and stored at 2-8 °C.
2. Secure the strips into the holding frame.
3. Pipette 50 µL of each Calibrator, Control and Sample into the appropriate wells.
4. Pipette 150 µL of Incubation Buffer into all the wells.
5. Incubate for 2 hours at room temperature, on a plate shaker (400 rpm). Prepare the Working HRP conjugate solution during the incubation and a minimum of 1 hour 45 minutes before its use.
6. Aspirate the liquid from each well.
7. Wash the plate 3 times by:
 - a. dispensing 0.35 mL of Working Wash solution into each well
 - b. aspirating the content of each well
8. Pipette 200 µL of the Working HRP conjugate solution into each well. Incubate the microplate for 30 minutes at room temperature, on a plate shaker (400 rpm).
9. Aspirate the liquid from each well.
10. Wash the plate 3 times by:
 - a. dispensing 0.35 mL of Working Wash solution into each well
 - b. aspirating the content of each well
11. Pipette 100 µL of the Chromogenic solution into each well within 15 minutes following the washing step.
12. Incubate the microplate for 15 minutes at room temperature, on a plate shaker (300 to 700 rpm), avoid direct sunlight.
13. Pipette 100 µL of Stop solution into each well.
14. Read the absorbance at 450 nm (reference filter 630 nm or 650 nm) within 1 hour and calculate the results as described in section XII.

XI. CALCULATION OF RESULTS

1. Read the plate at 450 nm against a reference filter set at 650 nm (or 630 nm).
2. Calculate the mean of duplicate determinations.
3. We recommend the use of computer assisted methods to construct the calibration curve. 4-parameter logistic function curve fitting is the preferred method. Reject obvious outliers.
4. By interpolation of the sample OD values, determine the 25-OH Vitamin D concentrations of the samples from the calibration curve.

XII. PERFORMANCE AND LIMITATIONS

A. Typical Data

The following data are for illustration only and should never be used instead of the real-time calibration curve.

25-OH ELISA		OD Units
Calibrator	0 ng/mL	2.66
	5.3 ng/mL	2.39
	15.0 ng/mL	1.83
	25.7 ng/mL	1.46
	54.3 ng/mL	0.81
	133 ng/mL	0.21

Note: 1 ng/mL=2.5 pmol/mL

B. Limits of Detection

The Limit of Blank (LoB), Limit of Detection (LoD), and the Limit of Quantitation (LoQ), were determined in accordance with the CLSI guideline EP17-A. The LoB was calculated by measuring the blank several times and calculating the 95th percentile of the distribution of the test values. The LoB was calculated to be 1.69 ng/mL. The LoD was calculated as described in the guideline. The LoD was calculated to be 2.81 ng/mL. The LoQ was calculated by testing 5 samples of low value 14 times in different tests. The LoQ was calculated to be 4.39 ng/mL with a CV of 20 %.

C. Performance Characteristics

Cross reactivity of the 25-OH Vitamin D Total ELISA assay was determined by testing sera with spiked and unspiked cross reactants. The results are summarized in the following table:

Compound and Concentration	% Cross reaction
25-OH-Vitamin D ₃ at 10 ng/mL	100
25-OH-Vitamin D ₂ at 10 ng/mL	86
1, 25(OH) ₂ -Vitamin D ₃ at 200 ng/mL	20
1, 25(OH) ₂ -Vitamin D ₂ at 690 ng/mL	1.9
Vitamin D ₃ at 200 ng/mL	2.9
Vitamin D ₂ at 200 ng/mL	1.3
24, 25(OH) ₂ -Vitamin D ₃ at 20 ng/mL	>100
25, 26(OH) ₂ -Vitamin D ₃ at 4 ng/mL	>100
3-epi-25-OH-Vitamin D ₃ at 20 µg/mL	0.1

The effect of potential interfering substances on samples using the Human 25-OH Total Vitamin D IVD ELISA Kit was evaluated. Different levels of Hemoglobin, Bilirubin Conjugated and Unconjugated, Triglyceride, Vitamin C, Biotin, and Zemplar in serum samples were tested on samples with different 25-OH Vitamin D concentrations. Our acceptance criterion was to have interference of less than 10 %. The tested substances did not affect the performance of the 25-OH Vitamin D Total ELISA Kit.

Substance	25-OH Vitamin D (ng/mL)	Concentration of Interferent (mg/dL)	Mean % Variation
Hemoglobin	7.6	250	-0.6 %
		500	
	29.3	250	
		500	
	42.5	250	
		500	
Bilirubin Conjugated	6.0	50	-3.4 %
		100	
	21.5	50	
		100	
	38.6	50	
		100	
Bilirubin Unconjugated	7.6	50	2.5 %
		100	
	29.3	50	
		100	
	42.5	50	
		100	
Triglyceride	7.6	7.5	-4.3 %
		125	
		250	
		500	
	29.3	7.5	
		125	
		250	
		500	
	42.5	7.5	
		125	
		250	
		500	

Substance	25-OH Vitamin D (ng/mL)	Concentration of Interferent (mg/dL)	Mean % Variation
Vitamin C	6.0	1	2.5 %
		10	
		100	
	21.5	1	
		10	
		100	
	38.6	1	
		10	
		100	
Biotin	8.7	0.2	4.7 %
		2	
		4	
	19.8	0.2	
		2	
		4	
	36.1	0.2	
		2	
		4	
Zemplar	17.6	0.0013	-4.4 %
		0.0025	
		0.0050	
	33.5	0.0013	
		0.0025	
		0.0050	

D. Precision

The assay precision was calculated by running samples for a span of at least 20 days on 3 different lots. The results are summarized in the table below:

Intra-Assay Precision				Inter-Assay Precision			
Sample	n	<X> ± SD (ng/mL)	C.V. (%)	Sample	n	<X> ± SD (ng/mL)	C.V. (%)
A	24	5.5 ± 0.4	7.8	A	39	17.7 ± 1.3	7.4
B	35	27.4 ± 1.6	5.7	B	10	26.3 ± 1.2	4.7
C	35	43.0 ± 1.2	2.7	C	10	42.1 ± 1.8	4.3
D	24	81.2 ± 2.0	2.5	D	21	85.4 ± 7.8	9.2

SD : Standard Deviation, CV: Coefficient of variation

E. Reproducibility

The reproducibility of the assay was done by testing three samples in duplicate for five days, twice a day, at three sites with two technicians per site. The mean results are summarized in the table below:

Sample	n	ng/mL		Within Run	Between Run	Between Day	Between Tech	Between Site	Total
1	57	25.5	SD	0.22	0.61	0.98	1.54	2.21	2.59
			CV	0.3 %	0.9 %	3.8 %	6.0 %	8.7 %	10.2 %
2	57	52.9	SD	0.64	1.57	1.11	2.28	4.29	5.19
			CV	0.9 %	2.3 %	2.1 %	4.3 %	8.1 %	9.8 %
3	59	124.9	SD	1.00	1.74	1.84	3.39	4.98	6.25
			CV	1.4 %	2.5 %	1.5 %	2.7 %	4.0 %	5.0 %

F. Accuracy

Recovery was assessed by adding different levels of 25-OH Vitamin D to samples. The results are summarized in the table below:

Recovery Test			
Added 25-OH-Vit.D ₃ (ng/mL)	Recovery (%)	Added 25-OH-Vit.D ₂ (ng/mL)	Recovery (%)
0	100	0	100
25	96	25	105
50	92	50	95

Two samples with concentrations known to be distributed throughout the measurable range were tested at equidistant dilutions to determine the linear range of the assay. A linear regression analysis was performed. The results are summarized in the following table:

Sample 1

Sample Dilution	Theoretical Concentration (ng/mL)	Measured Concentration (ng/mL)	Slope	Y-Intercept	R ²	Recovery (%)
1/1	96.7	96.7	1.00	-0.30	0.99	100
1/2	48.5	47.6				99
1/4	24.2	24.5				101
1/8	12.1	11.1				92
1/16	6.0	6.2				102

Sample 2

Sample Dilution	Theoretical Concentration (ng/mL)	Measured Concentration (ng/mL)	Slope	Y-Intercept	R ²	Recovery (%)
1/1	122.9	122.9	1.01	0.44	0.99	100
1/2	61.5	64.5				105
1/4	30.7	31.5				103
1/8	15.4	15.0				98
1/16	7.7	7.6				99

The linear range of the assay was found to be 7.7 ng/mL to 122.9 ng/mL.

G. Time delay


The results of the time delay test between the last Calibrator and sample dispensing are shown in the following table:

	Time Delay		
	0 min (ng/mL)	10 min (ng/mL)	20 min (ng/mL)
Sample 1	27.9	30.5	30.2
Sample 2	49.5	47.5	49.0

Assay results remain accurate even when Incubation Buffer is dispensed 10 and 20 minutes after the Calibrator has been added in the coated wells.

H. Method comparison

The performance of the Human Total 25-OH Vitamin D IVA ELISA Kit was determined by conducting a correlation study tested at three different sites using a total of 356 samples. The samples were tested on both the Human Total 25-OH Vitamin D IVA ELISA Kit and a commercially available 25-OH Vitamin D ELISA test. The results ranged from 8.0 ng/mL to 123.0 ng/mL, the correlation coefficient between the two methods was 0.917, with the 95 % confidence interval of 87.6 % to 93.6 %, a slope of 0.954 and the y-intercept of 3.05. The following graph summarizes the results:

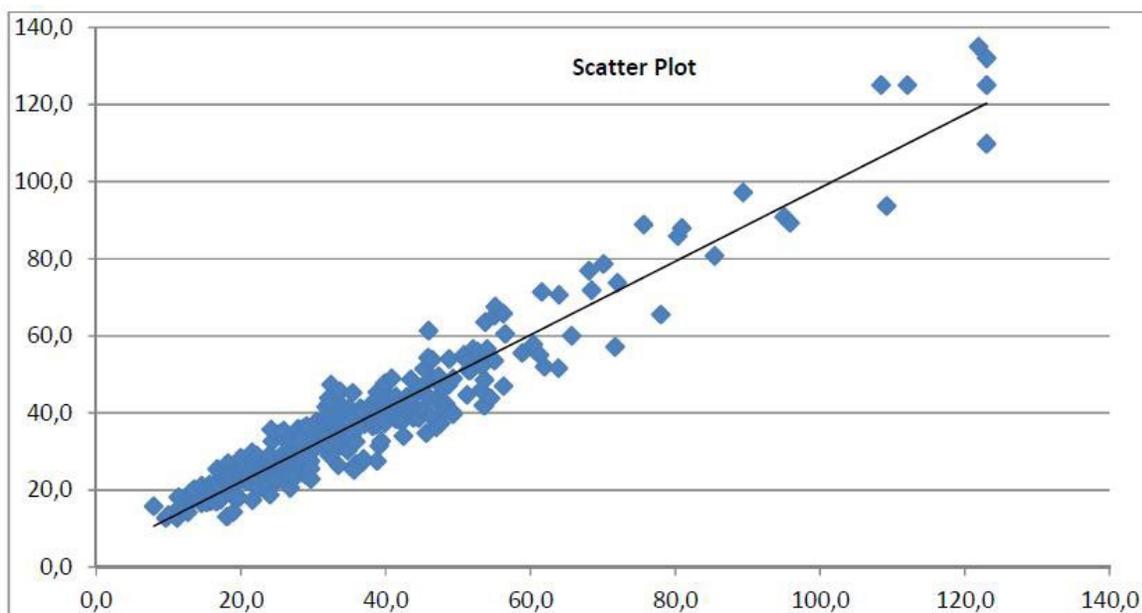

XIII. INTERNAL QUALITY CONTROL

- If the results obtained for Control 1 and/or Control 2 are not within the range specified on the vial label, the results cannot be used unless a satisfactory explanation for the discrepancy has been given.
- If desirable, each laboratory can make its own pools of control samples, which should be kept frozen in aliquots. Controls which contain azide will interfere with the enzymatic reaction and cannot be used.
- Acceptance criteria for the difference between the duplicate results of the samples should rely on Good Laboratory Practices.
- It is recommended that Controls be routinely assayed as unknown samples to measure assay variability. The performance of the assay should be monitored with quality control charts of the controls.
- It is good practice to check visually the curve fit selected by the computer.

XIV. EXPECTED VALUES

Dietary intake, race, season and age are known to affect the normal levels of 25-OH Vitamin D3. Each laboratory should establish its own range based on their local population.

Recent literature has suggested the following ranges for the classification of 25-OH Vitamin D status:

Level	ng/mL
Deficient	<10
Insufficient	10-29
Sufficient	30-100
Potential Toxicity	>100

Reference ranges have been established based on 150 apparently healthy individuals. The individual patient serum samples used were obtained from a certified commercial source and were collected from an FDA Licensed Donor Center with informed consent. 50 samples were from Northern US (Pennsylvania), 50 samples were from Central US (Tennessee), and 50 samples were from Southern US (Florida). Samples were collected in the winter months (January-March) from individuals between the ages of 21-92 years old and included both light skin and dark skin population. The donors from which samples were collected were not taking Vitamin D supplements, had no family history of parathyroid or calcium regulatory disease, had no history of kidney, liver, parathyroid, calcium related disease or bariatric surgery, and were not taking any medications known to affect absorption or catabolism of Vitamin D. The following table is the summary of results:

	Florida	Tennessee	Pennsylvania	Overall
Highest Conc. (ng/mL)	88.6	71.4	54.6	88.6
Lowest Conc. (ng/mL)	6.1	4.9	5.9	4.9
Median Conc. (ng/mL)	20.8	17.2	14.3	17.3

Only the central 95 % (2.5 % - 97.5 %) of the results observed were used.

XV. BIBLIOGRAPHY

1. ZERWEKH J.E. (2008) **Blood biomarkers of Vitamin D status.** Am. J. Clin. Nutr., 7(suppl):1087S-91S.
2. HOLICK M.F. (2006) **Resurrection of Vitamin D deficiency and rickets.** J. Clin. Invest., 116:2062-2072.
3. HEANEY R.P. (2000) **Vitamin D: how much do we need, and how much is too much.** Osteoporos. Int., 11:553-555.
4. DAWSON-HUGHES B., HEANEY R.P., HOLICK M.F., LIPS P., MEUNIER P.J. (1997) **Prevalence of Vitamin D insufficiency in an adult normal population.** Osteoporos. Int., 7:439-443.
5. BISCHOFF-FERRARI H.A., GIOVANNUCCI E., WILLETT W.C., DIETRICH T., DAWSON-HUGHES B. (2006) **Estimation of optimal serum concentrations of 25-hydroxyvitamin D for multiple health outcomes.** Am. J. Clin. Nutr., 84:18-28.
6. HOLICK M.F.(2004) **Sunlight and vitamin D for bone health and prevention of autoimmune diseases, cancers and cardiovascular disease.** Am. J. Clin. Nutr., 80:16788S-1688S.
7. HEANEY R.P. (2010) **Defining deficiency of vitamin D.** Clinical Laboratory International, October 2010, vol.34: 16-19.
8. HOLICK M.F. (2007) **Vitamin D deficiency.** N. Engl. J. Med., 357:266-281.
9. TAHA N. M. , VIETH R.(2010) **The problem of an optimal target level for 25-Hydroxyvitamin D, the test for vitamin D nutritional status.** Clinical Laboratory International , November 2010, vol.34 : 28-30
10. HOLICK M.F. (2009) **Vitamin D Status: Measurement, Interpretation, and Clinical Application.** Ann. Epidemiol., 19:73-78.
11. **National Osteoporosis Foundation. Prevention-Vitamin D**
<http://www.nof.org/aboutosteoporosis/prevention/vitamind>
12. EP17-A Protocols for Determination of Limits of Detection and Limits of Quantitation; Approved Guideline, STANDARD published by Clinical and Laboratory Standards Institute.

XVI. SUMMARY OF THE PROTOCOL

	Calibrators (uL)	Sample(s) Controls (uL)
Calibrators (0-5)	50	—
Controls, Samples	—	50
Incubation Buffer	150	150
<p>Incubate for 2 hours at room temperature with continuous shaking at 400 rpm.</p> <p>Prepare the Working HRP conjugate during the incubation and a minimum of 1 hour 45 minutes before its use (see section IX.D).</p> <p>Aspirate the contents of each well.</p> <p>Wash 3 times with 350 µL of Working Wash solution and aspirate.</p>		
Working HRP conjugate	200	200
<p>Incubate for 30 minutes at room temperature with continuous shaking at 400 rpm.</p> <p>Aspirate the contents of each well.</p> <p>Wash 3 times with 350 µL of Working Wash solution and aspirate.</p>		
Chromogenic solution	100	100
<p>Incubate for 15 min at room temperature with continuous shaking at 400 rpm.</p>		
Stop solution	100	100
<p>Read on a microplate reader.</p> <p>Record the absorbance of each well at 450 nm (versus 630 or 650 nm).</p>		