

# Human IL-10 ELISA Kit

Instructions for use

Catalogue numbers:	1x48 tests:	950.060.048
	1x96 tests:	950.060.096
	2x96 tests:	950.060.192

**For research use only**

Fast Track Your Research.....

## Table of Contents

1. Intended use .....	2
2. Introduction .....	2
2.1. Summary .....	2
2.2. Principle of the method .....	2
3. Reagents provided and reconstitution .....	3
4. Materials required but not provided .....	3
5. Storage Instructions .....	4
6. Specimen collection, processing & storage .....	4
7. Safety & precautions for use .....	5
8. Assay Preparation .....	6
8.1. Assay Design .....	6
8.2. Preparation of Wash Buffer .....	6
8.3. Preparation of Standard Diluent Buffer 1X .....	6
8.4. Preparation of Standard .....	7
8.5. Preparation of Control .....	7
8.6. Preparation of Biotinylated Anti-IL-10 .....	7
8.7. Preparation of Streptavidin-HRP .....	8
9. Method .....	9
10. Data Analysis .....	10
11. Assay limitations .....	10
12. Performance Characteristics .....	11
12.1. Sensitivity .....	11
12.2. Specificity .....	11
12.3. Precision .....	11
12.4. Dilution Parallelism .....	12
12.5. Spike Recovery .....	12
12.6. Stability .....	12
12.7. Expected serum values .....	12
12.8. Standard Calibration .....	12
13. Bibliography .....	13
14. Diaclone Human IL-10 ELISA references .....	13
15. Assay Summary .....	16

# Human IL-10 ELISA KIT

## 1. Intended use

The Diaclone Human IL-10 ELISA kit is a solid phase sandwich ELISA for the *in-vitro* qualitative and quantitative determination of IL-10 in supernatants, buffered solutions or serum and plasma samples. This assay will recognise both natural and recombinant human IL-10.

**This kit has been configured for research use only. Not suitable for use in therapeutic procedures.**

## 2. Introduction

### 2.1. Summary

Interleukin-10 is a pleiotropic cytokine playing an important role as a regulator of lymphoid and myeloid cell function. Due to the ability of IL-10 to block cytokine synthesis and several accessory cell functions of macrophages this cytokine is a potent suppressor of the effector functions of macrophages, T-cells and NK cells. In addition, IL-10 participates in regulating proliferation and differentiation of B-cells, mast cells and thymocytes (9). The primary structure of human IL-10 has been determined by cloning the cDNA encoding the cytokine (15). The corresponding protein exerts 160 amino acids with a predicted molecular mass of 18.5 kDa (8, 15). Based on its primary structure, IL-10 is a member of the four  $\alpha$ -helix bundle family of cytokines (11). In solution human IL-10 is a homodimer with an apparent molecular mass of 39 kDa (14). Although it contains an N-linked glycosylation site, it lacks detectable carbohydrates (15). Recombinant protein expressed in *E. coli* thus retains all known biological activities. The human IL-10 gene is located on chromosome 1 and is present as a single copy in the genome (6). The human IL-10 exhibits strong DNA and amino acid sequence homology to the murine IL-10 and an open reading frame in the Epstein- Barr virus genome, BCRF1 (1, 8, 15) which shares many of the cellular cytokine's biological activities and may therefore play a role in the host- virus interaction.

The immunosuppressive properties of IL-10 (4) suggest a possible clinical use of IL-10 in suppressing rejections of grafts after organ transplantations. IL-10 can furthermore exert strong anti-inflammatory activities (4).

### IL-10 in disease

IL-10 expression was shown to be elevated in **parasite infections** like in *Schistosoma mansoni* (7), *Leishmania* (5), *Toxoplasma gondii* (12) and *Trypanosoma* (13) infection. Furthermore, high IL-10 expression was detected in **mycobacterial infections** as shown for *Mycobacterium leprae* (3), *Mycobacterium tuberculosis* (2) and *Mycobacterium avium* infections. High expression levels of IL-10 are also found in **retroviral infections** inducing immunodeficiency (10).

### 2.2. Principle of the method

A capture Antibody highly specific for IL-10 has been coated to the wells of the microtiter strip plate provided during manufacture. Binding of IL-10 in samples and known standards to the capture antibodies is completed and then any excess unbound analyte is removed.

During the next incubation period the binding of the Biotinylated anti-IL-10 secondary antibody to the analyte occurs. Any excess unbound secondary antibody is then removed.

The HRP conjugate solution is then added to every well including the zero wells, following incubation excess conjugate is removed by careful washing.

A chromogen substrate is added to the wells resulting in the progressive development of a blue coloured complex with the conjugate. The colour development is then stopped by the addition of acid turning the resultant final product yellow. The intensity of the produced coloured complex is directly proportional to the concentration of IL-10 present in the samples and standards.

The absorbance of the colour complex is then measured and the generated OD values for each standard are plotted against expected concentration forming a standard curve. This standard curve can then be used to accurately determine the concentration of IL-10 in any sample tested.

### 3. Reagents provided and reconstitution

Reagents (Store @ 2-8°C)	Quantity 1x48-well kit Cat no. 950.060.048	Quantity 1x96-well kit Cat no. 950.060.096	Quantity 2x96-well kit Cat no. 950.060.192	Reconstitution
Anti-IL-10 Coated Plate	1/2	1	2	Ready to use (96-well strip pre-coated plate)
Plastic plate covers	2	2	4	n/a
IL-10 Standard: 400 pg/ml	1	2	4	Reconstitute as directed on the vial (see Assay preparation, section 8)
Standard Diluent (Buffer)	1 (15ml)	1 (15ml)	1 (25ml)	10x concentrate, dilute in distilled water (see Assay preparation, section 8)
Standard Diluent Serum	1 (7 ml)	1 (7 ml)	2 (7 ml)	Ready to use
IL-10 Control	1	2	4	Reconstitute as directed on the vial (see Assay preparation, section 8)
Biotinylated Anti-IL-10	1 (0.4ml)	1 (0.4ml)	2 (0.4ml)	Dilute in Biotinylated Antibody Diluent (see Assay preparation, section 8)
Biotinylated Antibody Diluent	1 (7ml)	1 (7ml)	1 (13ml)	Ready to use
Streptavidin-HRP	1 (5µl)	2 (5µl)	4 (5µl)	Add 0.5ml of Streptavidin-HRP Diluent prior to use (see Assay preparation, section 8)
Streptavidin-HRP Diluent	1 (12ml)	1 (12ml)	1 (23ml)	Ready to use
Wash Buffer	1 (10ml)	1 (10ml)	2 (10ml)	200x concentrate dilute in distilled water (see Assay preparation, section 8)
TMB Substrate	1 (11ml)	1 (11ml)	1 (24ml)	Ready to use
H <sub>2</sub> SO <sub>4</sub> Stop Reagent	1 (11ml)	1 (11ml)	2 (11ml)	Ready to use

### 4. Materials required but not provided

- Microtiter plate reader fitted with appropriate filters (450 nm required with optional 620 nm reference filter)
- Microtiter plate washer or wash bottle
- 10, 50, 100, 200 and 1,000µl adjustable single channel micropipettes with disposable tips
- 50-300µl multi-channel micropipette with disposable tips
- Multichannel micropipette reagent reservoirs
- Distilled water
- Vortex mixer
- Miscellaneous laboratory plastic and/or glass, if possible sterile

## 5. Storage Instructions

Store kit reagents between 2 and 8°C. Immediately after use remaining reagents should be returned to cold storage (2-8°C). Expiry of the kit and reagents is stated on box front labels. The expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, the reagent is not contaminated by the first handling.

**Wash Buffer 1X:** Once prepared, store at 2-8°C for up to 1 week.

**Standard Diluent Buffer 1X:** Once prepared, store at 2-8°C for up to 1 week.

**Reconstituted Standard/Control:** Once prepared use immediately and do not store.

**Diluted Biotinylated Anti-IL-10:** Once prepared use immediately and do not store.

**Diluted Streptavidin-HRP:** Once prepared use immediately and do not store.

## 6. Specimen collection, processing & storage

Cell culture supernatants, human serum, plasma or other biological samples will be suitable for use in the assay. Remove serum from the clot or red cells, respectively, as soon as possible after clotting and separation.

**Cell culture supernatants:** Remove particulates and aggregates by spinning at approximately 1000 x g for 10 min.

**Serum:** Use pyrogen/endotoxin free collecting tubes. Serum should be removed rapidly and carefully from the red cells after clotting. Following clotting, centrifuge at approximately 1000 x g for 10 min and remove serum.

**Plasma:** EDTA, citrate and heparin plasma can be assayed. Spin samples at 1000 x g for 30 min to remove particulates. Harvest plasma.

**Storage:** If not analysed shortly after collection, samples should be aliquoted (250-500µl) to avoid repeated freeze-thaw cycles and stored frozen at -70°C. Avoid multiple freeze-thaw cycles of frozen specimens.

**Recommendation:** Do not thaw by heating at 37°C or 56°C. Thaw at room temperature and make sure that sample is completely thawed and homogeneous before use. When possible avoid use of badly haemolysed or lipemic sera. If large amounts of particles are present these should be removed prior to use by centrifugation or filtration.

## 7. Safety & precautions for use

- Handling of reagents, serum or plasma specimens should be in accordance with local safety procedures, e.g. CDC/NIH Health manual: "Biosafety in Microbiological and Biomedical Laboratories" 1984.
- Laboratory gloves should be worn at all times.
- Avoid any skin contact with H<sub>2</sub>SO<sub>4</sub> and TMB. In case of contact, wash thoroughly with water.
- Do not eat, drink, smoke or apply cosmetics where kit reagents are used.
- Do not pipette by mouth.
- When not in use, kit components should be stored refrigerated as indicated on vials or bottles labels.
- All reagents should be warmed to room temperature before use. Lyophilized standards should be discarded after use.
- Once the desired number of strips has been removed, immediately reseal the bag to protect the remaining strips from deterioration.
- Cover or cap all reagents when not in use.
- Do not mix or interchange reagents between different lots.
- Do not use reagents beyond the expiration date of the kit.
- Use a clean disposable plastic pipette tip for each reagent, standard, or specimen addition in order to avoid cross contamination, for the dispensing of H<sub>2</sub>SO<sub>4</sub> and TMB Substrate solutions, avoid pipettes with metal parts.
- Use a clean plastic container to prepare the washing solution.
- Thoroughly mix the reagents and samples before use by agitation or swirling.
- All residual washing liquid must be drained from the wells by efficient aspiration or by decantation followed by tapping the plate forcefully on absorbent paper. Never insert absorbent paper directly into the wells.
- The TMB Substrate solution is light sensitive. Avoid prolonged exposure to light. Also, avoid contact of the TMB Substrate solution with metal to prevent colour development. Warning TMB Substrate is toxic avoid direct contact with hands. Dispose off properly.
- If a dark blue colour develops within a few minutes after preparation, this indicates that the TMB Substrate solution has been contaminated and must be discarded. Read absorbances within 1 hour after completion of the assay.
- When pipetting reagents, maintain a consistent order of addition from well-to-well. This will ensure equal incubation times for all wells.
- Follow incubation times described in the assay procedure.
- Dispense the TMB Substrate within 15 min of the washing of the microtiter plate.

## 8. Assay Preparation

Bring all reagents to room temperature before use

### 8.1. Assay Design

Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running zeros and standards. Each sample, standard, zero and control should be tested **in duplicate**. Remove sufficient microwell strips for testing from the pouch immediately prior to use. Return any wells not required for this assay with desiccant to the pouch. Seal tightly and return to 2-8°C storage.

**Example plate layout** (example shown for a 6 point standard curve)

	Standards / Controls		Sample Wells									
	1	2	3	4	5	6	7	8	9	10	11	12
A	400	400										
B	200	200										
C	100	100										
D	50	50										
E	25	25										
F	12.5	12.5										
G	zero	zero										
H	Ctrl	Ctrl										

*All remaining empty wells can be used to test samples in duplicate*

### 8.2. Preparation of Wash Buffer

If crystals have formed in the concentrate Wash Buffer, warm it gently until complete dissolution.

Dilute the (200X) concentrate Wash Buffer 200 fold with distilled water to give a 1X working solution. Pour entire contents (10 ml) of the concentrate Wash Buffer into a clean 2,000 ml graduated cylinder. Bring final volume to 2,000 ml with glass-distilled or deionized water. Mix gently to avoid foaming. Transfer to a clean wash bottle and store at 2°-25°C.

### 8.3. Preparation of Standard Diluent Buffer 1X

If crystals have formed in the concentrate Standard Diluent, warm it gently until complete dissolution.

Dilute the (10X) concentrate Standard Diluent 10 fold with distilled water to give a 1X working solution. Pour entire contents of the concentrate Standard Diluent into a clean appropriate graduated cylinder. Bring to final volume with glass-distilled or deionized water. Transfer to a clean wash bottle and store at 2°-25°C. Please see example volumes below:

Standard Diluent concentrate (ml)	Distilled water (ml)
15	135
25	225

## 8.4. Preparation of Standard

Depending on the type of samples you are assaying, the kit may include two Standard Diluents. Because biological fluids might contain proteases or cytokine-binding proteins that could modify the recognition of the cytokine you want to measure, you should reconstitute standard vials with the most appropriate Standard Diluent.

For **serum and plasma** samples: use Standard Diluent - Serum

For **cell culture supernatants**: use Standard Diluent Buffer 1X

Standard vials must be reconstituted with the volume of Standard Diluent shown on the vial immediately prior to use. This reconstitution gives a stock solution of 400 pg/ml of IL-10. Mix the reconstituted standard gently by inversion only. Serial dilutions of the standard are made directly in the assay plate to provide the concentration range from 400 to 12.5 pg/ml. A fresh standard curve should be produced for each new assay.

- Immediately after reconstitution add 200µl of the reconstituted standard to wells A1 and A2, which provides the highest concentration standard at 400 pg/ml.
- Add 100µl of Standard Diluent to the remaining standard wells B1 and B2 to F1 and F2.
- Transfer 100µl from wells A1 and A2 to B1 and B2. Mix the well contents by repeated aspirations and ejections taking care not to scratch the inner surface of the wells.
- Continue this 1:1 dilution using 100µl from wells B1 and B2 through to wells F1 and F2 providing a serial diluted standard curve ranging from 400pg/ml to 12.5pg/ml.
- Discard 100µl from the final wells of the standard curve (F1 and F2).

Alternatively these dilutions can be performed in separate clean tubes and immediately transferred into the relevant wells.

## 8.5. Preparation of Control

Freeze-dried control vials should also be reconstituted with the most appropriate Standard Diluent to your samples.

For **serum and plasma** samples: use Standard Diluent - Serum

For **cells culture supernatants**: use Standard Diluent Buffer 1X

The supplied Controls must be reconstituted with the volume of Standard Diluent indicated on the vial. Reconstitution of the freeze-dried material with the indicated volume, will give a solution at the concentration stated on the vial. Do not store after use.

## 8.6. Preparation of Biotinylated Anti-IL-10

It is recommended this reagent is prepared immediately before use. Dilute the Biotinylated Anti-IL-10 with the Biotinylated Antibody Diluent in an appropriate clean glass vial using volumes appropriate to the number of required wells. Please see example volumes below:

Number of wells required	Biotinylated Antibody (µl)	Biotinylated Antibody Diluent (µl)
16	40	1060
24	60	1590
32	80	2120
48	120	3180
96	240	6360



## 8.7. Preparation of Streptavidin-HRP

It is recommended to centrifuge vial for a few seconds in a microcentrifuge to collect all the volume at the bottom.

Dilute the 5 $\mu$ l vial with 0.5ml of Streptavidin-HRP Diluent **immediately before use**. Do not keep this diluted vial for future experiments. Further dilute the HRP solution to volumes appropriate for the number of required wells in a clean glass vial. Please see example volumes below:

Number of wells required	Streptavidin-HRP ( $\mu$ l)	Streptavidin-HRP Diluent (ml)
16	30	2
24	45	3
32	60	4
48	75	5
96	150	10

## 9. Method

We strongly recommend that every vial is mixed thoroughly without foaming prior to use.

Prepare all reagents as shown in section 8.

**Note:** final preparation of Biotinylated Antibody (section 8.6) and Streptavidin-HRP (section 8.7) should occur immediately before use.

Assay Step		Details
1.	Addition	<b>Prepare standard curve</b> as shown in section 8.4 above and add in duplicate to appropriate wells
2.	Addition	Add 100µl of each <b>Sample, Control and zero (appropriate Standard Diluent)</b> in duplicate to appropriate number of wells
3.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for <b>1 hour</b>
4.	Wash	Remove the cover and wash the plate as follows: a) Aspirate the liquid from each well b) Dispense 0.3 ml of <b>1x Wash Buffer</b> into each well c) Aspirate the contents of each well d) Repeat step b and c another two times
5.	Addition	Add 50µl of diluted <b>Biotinylated Anti-IL-10</b> to all wells
6.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for <b>1 hour</b>
7.	Wash	Repeat wash step 4.
8.	Addition	Add 100µl of diluted <b>Streptavidin-HRP</b> solution into all wells
9.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for <b>30 min</b>
10.	Wash	Repeat wash step 4.
11.	Addition	Add 100µl of ready-to-use <b>TMB Substrate</b> solution into all wells
12.	Incubation	Incubate in the dark for <b>10-15 minutes*</b> at room temperature. Avoid direct exposure to light by wrapping the plate in aluminium foil.
13.	Addition	Add 100µl of <b>H<sub>2</sub>SO<sub>4</sub> Stop Reagent</b> into all wells
<b>Read the absorbance</b> value of each well (immediately after step 13.) on a spectrophotometer using 450 nm as the primary wavelength and optionally 620 nm as the reference wave length (610 nm to 650 nm is acceptable).		

*\*Incubation time of the TMB Substrate is usually determined by the ELISA reader performance. Many ELISA readers only record absorbance up to 2.0 O.D. Therefore the colour development within individual microwells must be observed by the analyst, and the substrate reaction stopped before positive wells are no longer within recordable range.*

## 10. Data Analysis


Calculate the average absorbance values for each set of duplicate standards, control and samples. Ideally duplicates should be within 20% of the mean.

Generate a linear standard curve by plotting the average absorbance of each standard on the vertical axis versus the corresponding IL-10 standard concentration on the horizontal axis.

The amount of IL-10 in each sample is determined by extrapolating OD values against IL-10 standard concentrations using the standard curve.

### Example IL-10 Standard curve

Standard	IL-10 Conc (pg/ml)	OD (450nm) mean	CV (%)
1	400	2.559	0.64
2	200	1.416	0.71
3	100	0.862	0.86
4	50	0.454	0.91
5	25	0.286	1.14
6	12,5	0.180	1.44
zero	0	0.072	-

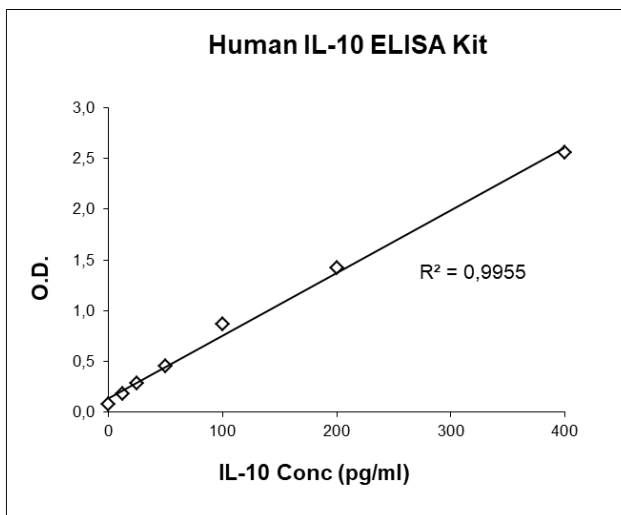

**Note:** curve shown above should not be used to determine results. Every laboratory must produce a standard curve for each set of microwell strips assayed.

## 11. Assay limitations

Do not extrapolate the standard curve beyond the maximum standard curve point. The dose-response is non-linear in this region and good accuracy is difficult to obtain. Concentrated samples above the maximum standard concentration must be diluted with Standard Diluent Buffer or with your own sample buffer to produce an OD value within the range of the standard curve. Following analysis of such samples always multiply results by the appropriate dilution factor to produce actual final concentration.

The influence of various drugs on end results has not been investigated. Bacterial or fungal contamination and laboratory cross-contamination may also cause irregular results.

Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing fresh Wash Buffer, fill with Wash Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.

As with most biological assays conditions may vary from assay to assay therefore **a fresh standard curve must be prepared and run for every assay.**

## 12. Performance Characteristics

### 12.1. Sensitivity

The sensitivity or minimum detectable dose of IL-10 using this Diaclone Human IL-10 ELISA kit was found to be **4.9pg/ml**. This was determined by adding 3 standard deviations to the mean OD obtained when the zero standard was assayed in 39 times.

### 12.2. Specificity

The assay recognizes both natural and recombinant human IL-10. To define the specificity of this ELISA several proteins were tested for cross reactivity. There was no cross reactivity observed for any protein tested: IL-1 $\beta$ , IL-2, IL-4, IL-6, IL-8, IL-12, IL-13, IL-17A, IFN $\gamma$  and TNF $\alpha$ .

### 12.3. Precision

#### Intra-assay

Reproducibility within the assay was evaluated in three independent experiments. Each assay was carried out with 6 replicates (3 duplicates) of samples containing different concentrations of IL-10: 2 in human pooled serum, 2 in culture media and 2 in standard diluent. Data below show the mean IL-10 concentration and the coefficient of variation for each sample.

**The calculated overall coefficient of variation was 3.5%.**

Session	Sample	Mean IL-10 pg/ml	SD	CV%
Session 1	Sample 1	226.14	2.41	1.07
	Sample 2	161.75	2.62	1.62
	Sample 3	304.46	11.95	3.93
	Sample 4	200.15	6.17	3.08
	Sample 5	209.90	13.80	6.57
	Sample 6	128.01	8.00	6.25
Session 2	Sample 1	225.88	0.25	0.11
	Sample 2	150.97	2.30	1.52
	Sample 3	304.57	28.76	9.44
	Sample 4	185.07	7.71	4.17
	Sample 5	212.52	10.44	4.91
	Sample 6	123.81	3.55	2.87
Session 3	Sample 1	172.89	7.84	4.54
	Sample 2	124.87	4.21	3.37
	Sample 3	254.52	1.35	0.53
	Sample 4	160.08	3.28	2.05
	Sample 5	174.57	4.42	2.53
	Sample 6	110.17	5.40	4.90

## Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in three independent experiments. Each assay was carried out with 6 replicates (3 duplicates) of samples containing different concentrations of IL-10: 2 in human pooled serum, 2 in culture media and 2 in standard diluent. Data below show the mean IL-10 concentration and the coefficient of variation for each sample.

**The calculated overall coefficient of variation was 7.5%.**

	<b>Sample 1</b>	<b>Sample 2</b>	<b>Sample 3</b>	<b>Sample 4</b>	<b>Sample 5</b>	<b>Sample 6</b>
<b>Mean IL-10 pg/ml</b>	220	154	308	194	212	129
<b>SD</b>	14	11	24	15	16	11
<b>CV%</b>	<b>6.4</b>	<b>6.8</b>	<b>7.8</b>	<b>7.9</b>	<b>7.5</b>	<b>8.3</b>

## 12.4. Dilution Parallelism

In two independent experiments two spiked human serum samples with different levels of IL-10 were analysed at different serial two fold dilutions (1:2 to 1:8) with two replicates each.

Recoveries ranged from 84 to 130% with an overall **mean recovery of 116%**.

## 12.5. Spike Recovery

The spike recovery was evaluated by spiking 2 concentrations of IL-10 in human serum and culture medium in 3 separate experiments.

Recoveries ranged from 83 to 122% with an overall **mean recovery of 103%**.

## 12.6. Stability

### Storage Stability

Aliquots of spiked serum and spiked medium were stored at  $-20^{\circ}\text{C}$ ,  $+2-8^{\circ}\text{C}$ , room temperature (RT) and at  $37^{\circ}\text{C}$  and the IL-10 level determined after 24h. There was no significant loss of IL-10 reactivity during storage at RT and  $2-8^{\circ}\text{C}$ , however there is a significant loss of reactivity when stored at  $37^{\circ}\text{C}$ .

### Freeze-thaw Stability

Aliquots of spiked serum and spiked medium were stored frozen at  $-20^{\circ}\text{C}$  and thawed up to 5 times and the IL-10 level was determined. There was no significant loss of IL-10 reactivity after 5 cycles of freezing and thawing.

## 12.7. Expected serum values

A panel of 20 human sera and 20 Plasma samples were tested for IL-10. All were below the detection level  $<4.9\text{pg/ml}$ .

## 12.8. Standard Calibration

This immunoassay is calibrated against the International Reference Standard NIBSC 93/722. NIBSC 93/722 is quantitated in International Units (IU). It has been calculated that 1 IU NIBSC correspond to 540pg Diaclone IL-10.

### 13. Bibliography

1. Baer R. and al, Nature. 1984 Jul 19-25;310(5974):207-11
2. Barnes P. and al, J Immunol. 1992 Jul 15;149(2):541-7.
3. Bloom B. and al, Immunol Rev. 1984 Aug;80:5-28.
4. De Waal Malefyt R. and al, J Exp Med. 1991 Nov 1;174(5):1209-20.
5. Heinzel F. and al, Proc Natl Acad Sci U S A. 1991 Aug 15;88(16):7011-5.
6. Kim J. and al, J Immunol. 1992 Jun 1;148(11):3618-23.
7. Kullberg M. and al, J Immunol. 1992 May 15;148(10):3264-70.
8. Moore K. and al, Science. 1990 Jun 8;248(4960):1230-4.
9. Moore K. and al, Annu Rev Immunol. 1993;11:165-90.
10. Mosier D. and al, J Exp Med. 1985 Apr 1;161(4):766-84.
11. Shanafelt A. and al, EMBO J. 1991 Dec;10(13):4105-12.
12. Sher A. and al, Immunol Rev. 1992 Jun;127:183-204.
13. Silva J. and al, J Exp Med. 1992 Jan 1;175(1):169-74.
14. Spits H. and al, Int Arch Allergy Immunol. 1992;99(1):8-15.
15. Vieira P. and al, Proc Natl Acad Sci U S A. 1991 Feb 15;88(4):1172-6.

### 14. Diacclone Human IL-10 ELISA references

1. Abbal C. et al., Int. Immunol., 1999; 11(9) : 1451 – 1462
2. Agahi, A. et al., Front Neurol. 2018 Aug 15;9:662
3. Akbari, F. et al., Iran J Neurol.,2016; 15(2): 75-9.
4. Altokka-Uzun, G. et al., Cephalalgia, 2015: 333102415570762
5. Bellanger, A.-P. et al., Clin. Vaccine Immunol., 2013 ; 20(8): 1133-1142.
6. Beyth S. et al., Blood, 2005; 105(5): 2214 – 2219
7. Biswas, S. et al., Korean J Intern Med.,2010 ; 25(1): 44-50
8. Calabro, M. L. et al., Blood,2009; 113(19): 4525-4533.
9. Cerkiene, Z. et al., Am J Reprod Immunol., 2008; 59(2): 118-26.
10. Chabbert-de Ponnat, I. et al., Int Immunol.,2005; 17(4): 439-47.
11. Chang, Y. et al.,FASEB J.,2010; Dec;24(12):5063-72
12. Charbonnier, A. S. et al., J Leukoc Biol.,2003; 73(1): 91-9.
13. Chavushyan, A. et al.,Schizophr Res Treatment,2013: 125264
14. Chen, Z. Q. et al.,World J Gastroenterol.,2004; 10(20): 3021-5.
15. Chenivresse, C. et al., J. Immunol.,2012; 189(1): 128-137
16. Cohen, N. et al., Blood,2006;107(5): 2037-44.
17. Corvaisier, M. et al., PLoS Biol.,2012;10(9): e1001395
18. Cunin, P. et al., J. Immunol.,2011;186(7): 4175-4182.
19. Das, A. et al., J. Immunol.,2012;189:3925-3935
20. de Nadai, P. et al., J Immunol.,2006;176(10): 6286-93.
21. Dominguez-Bernal, G. et al., Parasit Vectors,2015; 8: 629
22. Doniz-Padilla, L. et al., Eur. J. Endocrinol.,2011 ; 165(1): 129-136
23. El-Emshaty, H. M. et al., Dis Markers, 2015: 707254
24. Escolano, A. et al., Embo J.,2014;33(10): 1117-33
25. Fernandez-Yunquera, A. et al.,World J Transplant,2014; 4(2): 133-40
26. Forsbach, A. et al., J. Immunol.,2008;180(6): 3729-3738.
27. Foucher, E. D. et al., PLoS One,2013 ; 8(2): e56045
28. Fu, J. F. et al.,World J Gastroenterol.,2009;15(8):912-8
29. Gaayeb, L. et al., Am J Trop Med Hyg.,2014 ; 90(3): 566-573
30. Gary-Gouy H. et al., Blood, 2002; 100(13): 4537 – 4543
31. Gombocz, K. et al., Crit Care,2007; 11(4): R87
32. Gosset P. et al., J. Immunol., 2003 ; 170(10):4943 – 4952
33. Gu, Z. J. et al., Blood,1996; 88(10): 3972-86.
34. Hamdi, H. et al., Blood,2007; 110: 211 – 219
35. Hatzfeld-Charbonnier, A. S. et al., J Leukoc Biol.,2007;81: 1179 – 1187
36. Hernandez, C. et al., PLoS One,2014 ; 9(6): e98458
37. Holder, B. et al.,Traffic,2016 ;17(2):168-78

38. Iida, K. et al., *Oncol Lett.* 2019 Apr;17(4):4004-4010.
39. Iwamoto, S. et al., *J Leukoc Biol.*,2005;78(2): 383-92.
40. Jain, S. et al., *J. Med. Microbiol.*,2009; 58(2): 180-184.
41. Jimeno, R. et al., *J Mol Med. (Berl)*,2015; 93(4): 457-67
42. Jimeno, R. et al.,*J. Leukoc. Biol.*,2015 ; 98(2): 257-269
43. Jouan, J. et al., *J. Thorac. Cardiovasc. Surg.*, 2012;144(2):467-4732
44. Kayaba, H. et al., *J Immunol.*,2001; 167(2): 995-1003.
45. Kerblat, I. et al.,*Immunology*,2000; 100(2): 178-84.
46. Kerr J. et al., *J. Gen. Virol.*, 2001; 82(Pt 12): 3011-3019
47. Krasimirova, E. et al., *World J Exp Med.*, 2017 Aug 20;7(3):84-96.
48. Kumpf, O. et al. ,*Crit Care*,2010; 14(3): R103.
49. Kurowski, M. et al.,*Arch Med Sci.* 2018 Jan;14(1):60-68.
50. Kwan, W. H. et al., *J Leukoc Biol.*,2007; 82: 133 – 141
51. Kyriakopoulou, M. et al., *Mediators Inflamm.*, 2008: 450196.
52. Laborel-Preneron, E. et al.,*PLoS One*,2015; 10(10): e0141067
53. Lasisi, T. J. and A. F. Adeniyi, *Afr Health Sci.*,2016; 16(2): 560-6.
54. Liao, B. et al., *Emerg Microbes Infect.*,2015; 4(4): e24
55. Lieblein, J. C. et al.,*BMC Cancer*,2008; 8: 302
56. Llorente, L. et al., *Arthritis Rheum.*,2000; 43(8): 1790-800.
57. Loo, W. T. et al.,*J Transl Med.*,2012 10 Suppl 1: S8
58. Lopez-Abente, J. et al.,*Cell Mol Immunol.* 2018 Oct;15(10):917-933
59. Lu, C. et al., *Lupus*, 2015;24(1):18-24
60. Lu, Z. Y. et al., *FEBS Lett.*,1995; 377(3): 515-8.
61. Madej, M. et al., *Reumatologia*,2015; 53(1): 9-13.
62. Madempudi, R.S. et al.,*Sci Rep.* 2019 Aug 21;9(1):12210.
63. Mallick, B. et al., *JGH Open.* 2019 Mar 12;3(4): 295-301.
64. Mateen, S. et al.,*PLoS One.* 2017 Jun 8;12(6):e0178879
65. Moniuszko, M. et al.,*Inflammation*,2014;37(6): 1945-56
66. Montes, C. L. et al.,*Cancer Res.*,(2008; 68(3): 870-879.
67. Moreaux, J. et al., *Blood*,2011; 117(4): 1280-1290
68. Musleh, G. S. et al.,*Eur. J. Cardiothorac. Surg.*,2009; 35(3): 511-514.
69. Naisbitt D.J. et al., *J. Pharmacol. Exp. Ther.*, 2005; 313(3): 1058 – 1065
70. Naisbitt, D. J. et al., *Mol Pharmacol.*,2003; 63(3): 732-41.
71. Nayebifar, S. et al., *J Res Med Sci.*,2016; 21: 116.
72. Oksenhendler E. et al., *Blood*, 2000; 96(6): 2069 – 2073
73. Olivar, R. et al., *J. Immunol.*,2016;196(10): 4274-4290
74. Owczarczyk-Saczonek, A. et al.,*Postepy Dermatol Alergol.* 2019 Jun;36(3):319-328.
75. Paduch, R. et al., *Balkan Med J.*,2014;31(1): 29-36
76. Pene, J. et al., *J. Immunol.*,2008; 180(11): 7423-7430.
77. Perez S A. et al., *Blood*, 2003; 101(9): 3444 – 3450
78. Perez S. A. et al., *Blood*, 2005; 106(1):158 – 166
79. Perez, S. A. et al., *Clin Cancer Res.*,2007; 13(9): 2714-21.
80. Perez, S. A. et al., *Int Immunol.*,2006; 18(1): 49-58.
81. Perez-Bercoff D. et al., *J. Virol.*, 2003; 77(7): 4081 – 4094
82. Pichavant, M. et al., *J Immunol.*,2006; 177(9): 5912-9.
83. Plant, L. J. and A. B. Jonsson, *Infect Immun.*,2006; 74(1): 442-8.
84. Polz-Dacewicz, M. et al., *Infect Agent Cancer*,2016; 11: 45.
85. Rajappa, M. et al., *Angiology*,2009; 60(4): 419-426.
86. Rajbhoj, P. H. et al., *J Clin Diagn Res.*,2015; 9(2): CC01-5
87. Ralph, C. et al.,*Clin. Cancer Res.*,2010;16(5): 1662-1672
88. Rana, S. V. et al., *J Crohns Colitis*,2014 ; 8(8): 859-865
89. Ratajczak, C. et al., *J Biomed Biotechnol.*, 2007(1): 71921
90. Riccio, A. M. et al., *PLoS One*,2012; 7(6): e37980
91. Rodriguez-Zapata, M. et al., *Infect. Immun.*,2010; 78:3272-3279
92. Sadik, C. D. et al.,*Nucleic Acids Res.*,2009;gkp525.
93. Saverino D. et al., *J. immunol.*, 2002; 168(1): 207 – 215
94. Schiff-Zuck, S. et al., *J Immunol.*,2006; 177(11): 8241-7.
95. Schmitt, C. et al., *J Leukoc Biol.*,2000; 68(6): 836-44.
96. Schneider E M. et al., *Blood*, 2002; 100(8): 2891 – 2898

97. Segquier, S. et al., PLoS One,2013 ; 8(8): e70937
98. Sun, Z. et al., J Biomed Res.,2012; 26(6): 456-66
99. Tang, Y. et al., Am J Trop Med Hyg.,2008; 79(2): 154-158.
100. Tang, Y. et al.,PLoS One,2010 5(12): e15631
101. Valdor, R. et al.,Oncotarget. 2017 Aug 2;8(40):68614-68626.
102. Verghese, B. et al., Indian J Clin Biochem.,2011 ; 26(4): 373-7
103. Versaci, F. et al., Mayo Clin Proc.,2012; 87(1): 50-8
104. Vollmer J. et al., Antimicrob. Agents Chemother., 2004; 48(6): 2314 – 2317
105. Vollmer J. et al., J. Leukoc. Biol., 2004; 76(3): 585 – 593
106. Vollmer, J. et al.,Immunology,2004; 113(2): 212-23.
107. Woerly G. et al., J. Exp. Med., 1999; 190(4): 487 – 495
108. Zhang, Y. et al., Lupus, 2011; 20: 1172 – 1181
109. Ziesche, E. et al.,Clin Exp Immunol.,2009; 157(3): 370-6.



## 15. Assay Summary

Total procedure length: 2h45min

Add 100µl of Samples, Control and diluted Standards



Incubate 1 hour at room temperature



Wash three times



Add 50µl of diluted Biotinylated Antibody



Incubate 1 hour at room temperature



Wash three times



Add 100µl of diluted Streptavidin-HRP



Incubate 30 min at room temperature



Wash three times



Add 100µl of TMB Substrate  
Protect from light. Let the color develop for 10-15 min.



Add 100µl of Stop Reagent



Read Absorbance at 450 nm

### Products Manufactured and Distributed by:

Diaclone SAS  
6 Rue Docteur Girod  
25020 Besançon Cedex  
France  
Tel +33 (0)3 81 41 38 38  
Fax +33 (0)3 81 41 36 36  
Email: [info@diacclone.com](mailto:info@diacclone.com)